AQT0032 – ABL1 [H396P] Assay Validation

PhosphoSens®-Kinetic Assay Format

Outline for this Study

PhosphoSens-Kinetic Assay Validation

AssayQuant TECHNOLOGIES INC.

Enzyme Source, Construct, and Lot Information:

SignalChem ABL1 [H396P] (Cat#/Lot#: A03-12LG/U1510-5) amino acids 27-end; N-terminal GST-tag

Reference Compound Information:

Staurosporine MedChem Express

Experiments to be run:

Enzyme Titration

Sensor Peptide K_m Determination

ATP K_m Determination

DMSO Tolerance Test

Reference Compound IC_{50} Determination at ATP K_m

Enzyme Titration

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

15 µM AQT0032

0, 0.001, 0.002, 0.0039, 0.0078, 0.016, 0.031, 0.063, 0.13, 0.25, 0.50, 1 nM ABL1 [H396P]

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 or 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.

Notes:


Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


Enzyme Titration

Progress Curves


AssayQuant TECHNOLOGIES INC.


Complete Progress Curves

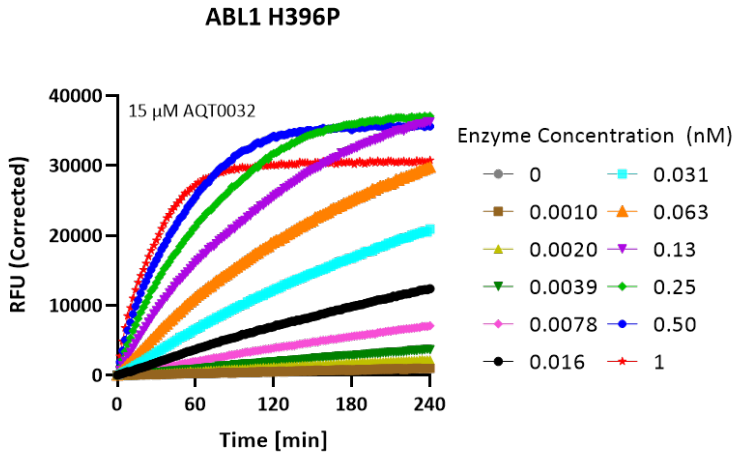

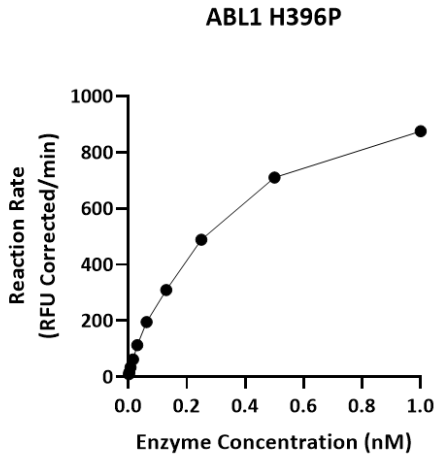

Linear Region of Progress Curves

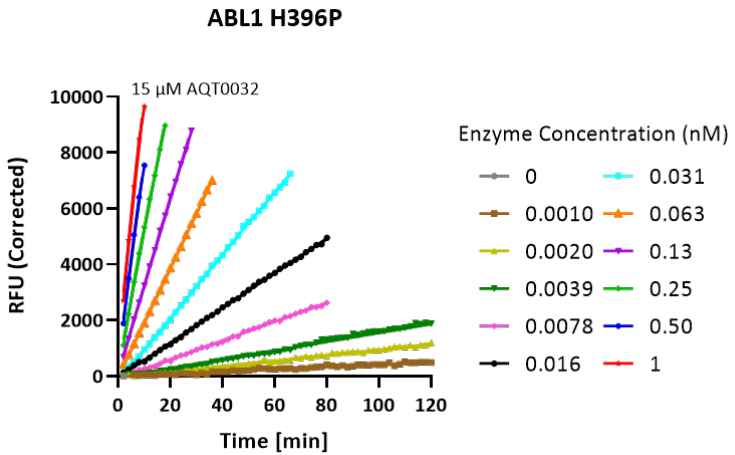

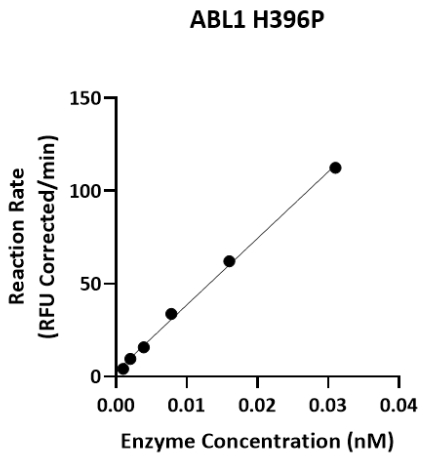

Linear Range

Enzyme Titration

Reaction Rate Table

Enzyme Conc. (nM)	Reaction Rate (RFU/min)	Normalized Reaction Rate (RFU/pmole/min)
0.001	4.2	210050
0.002	9.6	239725
0.0039	16	203333
0.0078	34	216795
0.016	62	194344
0.031	113	181452
0.063	195	155079
0.13	310	119192
0.25	489	97800
0.5	711	71070
1	876	43775

The reaction is linear from 0.001 - 0.31 nM

Sensor Peptide K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

0, 0.20, 0.39, 0.78, 1.6, 3.1, 6.3, 13, 25, 50, 100, and 200 µM AQT0032

0.02 nM ABL1 [H396P]

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


Sensor Peptide K_m Determination

Titration Curves and K_m Plot and Table

Sensor Peptide Titration Curves

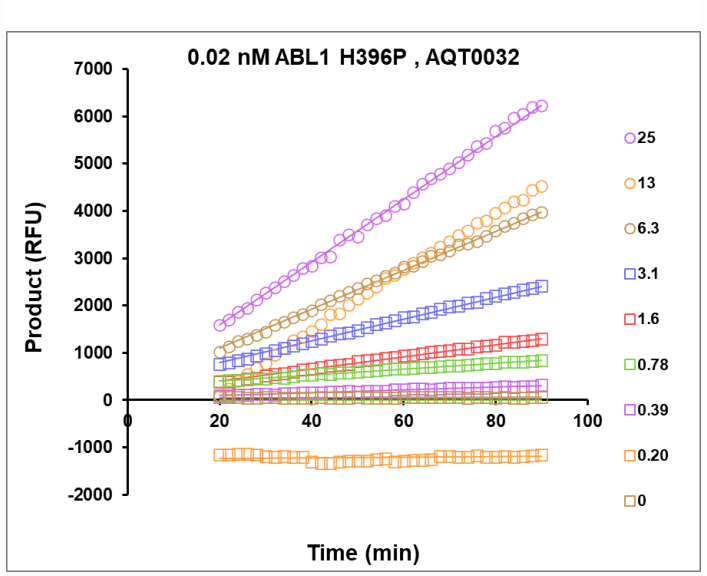

Sensor Peptide K_m Plot

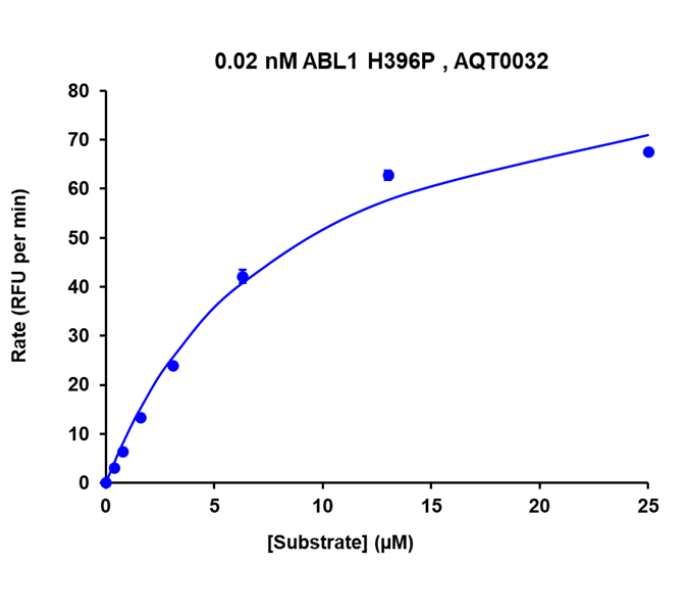

Sensor Peptide K_m Table

Parameter	Value	Approx SE
Vmax (RFU per min)	94.6	3.4
Vmax (RFU per pmol per min)	236398	8388
Km (µM)	8.3	0.1
R squared	0.990	

Sensor Peptide K_m is 8.3 µM

ATP K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

0, 2.0, 3.9, 7.8, 16, 31, 63, 125, 250, 500, 1000, and 2000 µM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

15 µM AQT0032

0.02 nM ABL1 [H396P]

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


ATP K_m Determination

Titration Curves and K_m Plot and Table

ATP Titration Curves

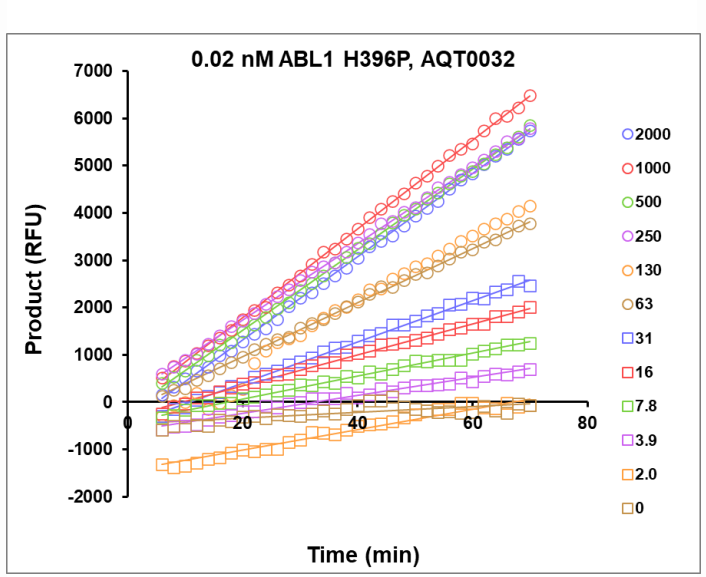

ATP K_m Plot

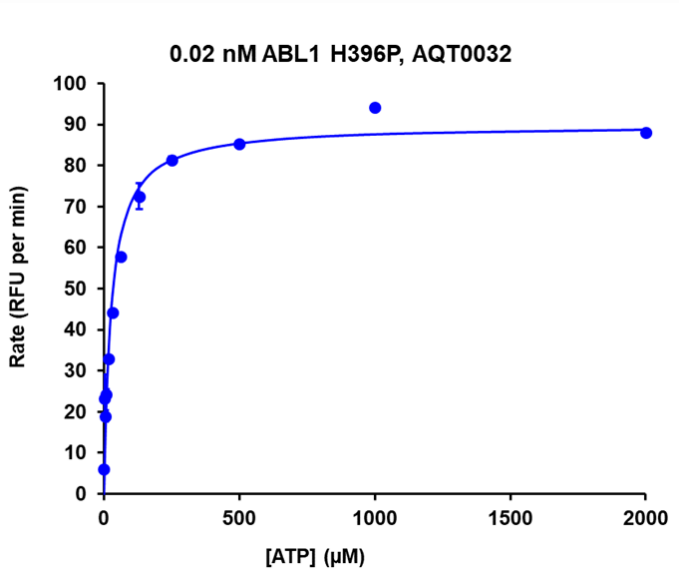

ATP K_m Table

Parameter	Value	Approx SE
Vmax (RFU per min)	90.0	1.5
Vmax (RFU per pmol per min)	224876	3840
Km (µM)	26.5	5.4
R squared	0.960	

ATP K_m is 27 µM

DMSO Tolerance Test

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

0, .01, .02, .04, .08, .16, .31, .63, 1.3, 2.5, 5.0, and 10% DMSO

15 µM AQT0032

0.01 nM ABL1 [H396P]

Reaction Set Up:

2 or 2.5 µL	10x DMSO dilutions
14 or 17.5 µL	Reaction Mix with Sensor Peptide, ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


DMSO Tolerance Test

Titration Curves and Inhibition Plot

Complete Progress Curves

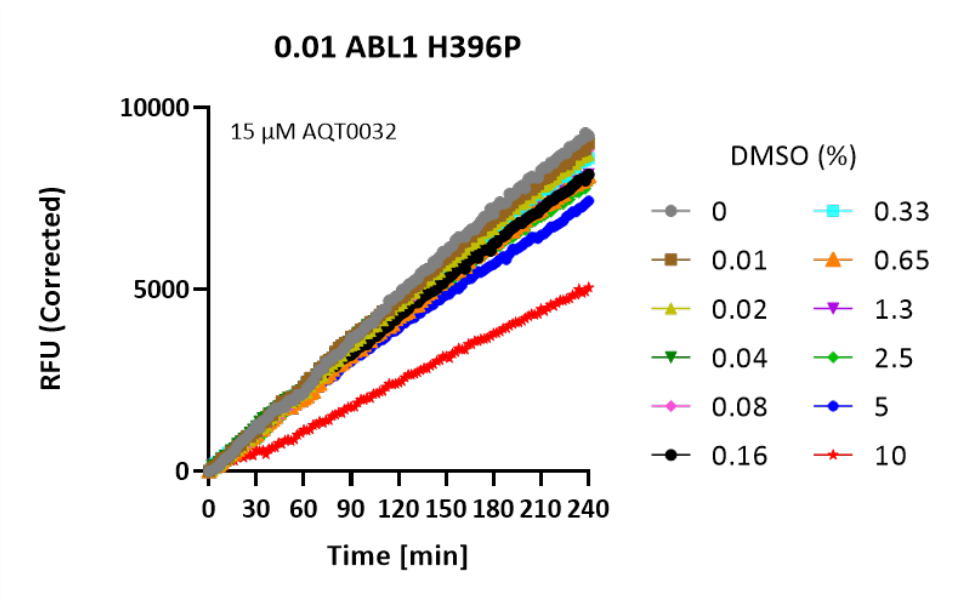

Reaction Rate vs [DMSO] Plot

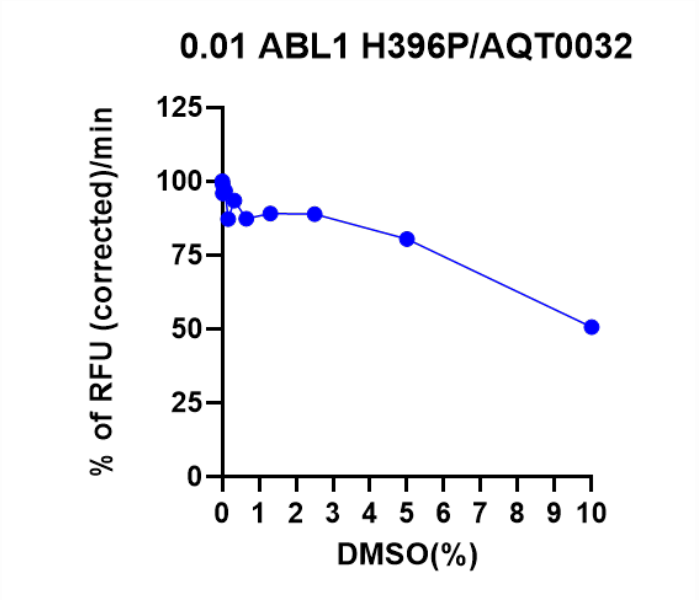

No change in enzyme activity out to 2% DMSO

IC_{50} Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

ATP at K_m

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

2% DMSO

15 µM AQT0032

0.03 nM ABL1 [H396P]

0, 0.0169, 0.0508, .152, .457, 1.37, 4.12, 12.3, 37, 111, 333, and 1000 nM Staurosporine

Reaction Set Up:

16 µL	Reaction Mix with Sensor Peptide and Inhibitor
4 µL	1x EDB or Kinase dilutions (5x in EDB)
20 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.

Inhibitors are added via direct (0.4 µL of 50X stock in 100% DMSO) or intermediate dilutions (2.0 µL of 10X stock in 10% DMSO).


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


IC_{50} Determination

Progress Curves and IC_{50} Curves and Table


Inhibitor Titration Progress Curves

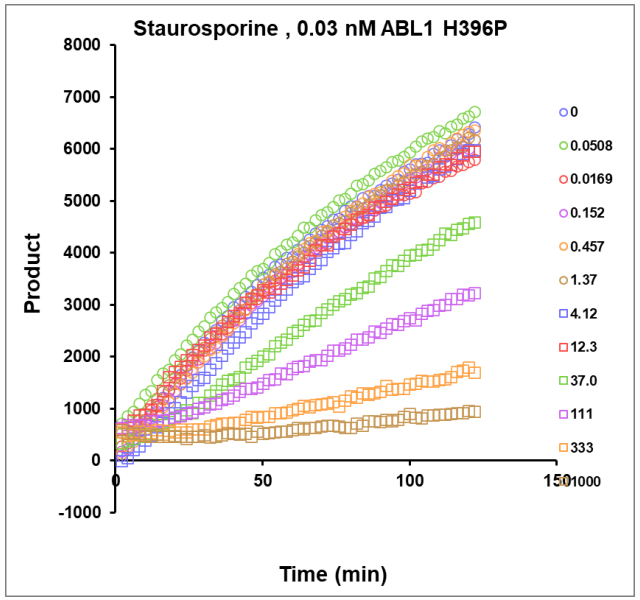

Linear Region of Progress Curves

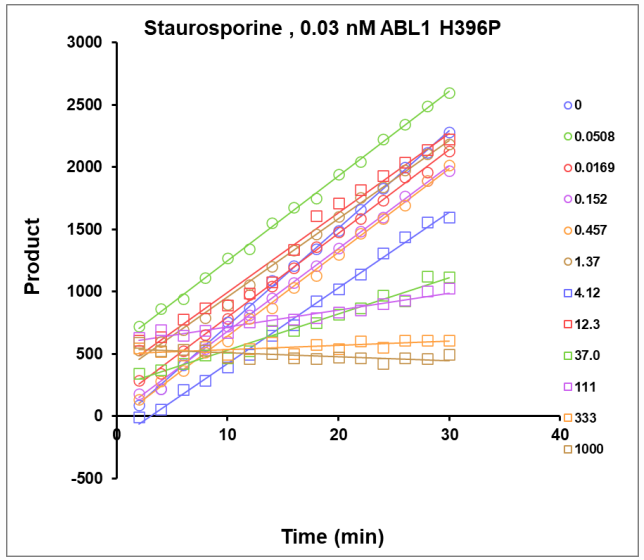

IC_{50} Curve

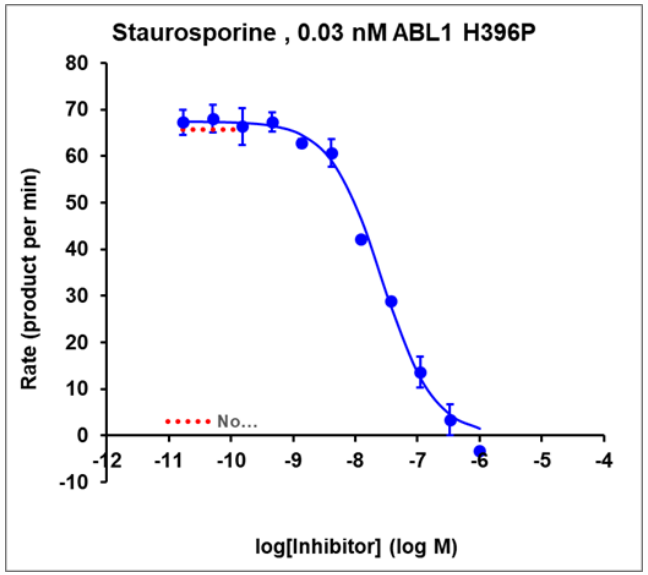

IC_{50} Table

Parameter	Value
Bottom	0.0
Top	67.3
log IC50	-7.58
IC50 (nM)	26.40
Ki (nM)	0.68
Slope	-1.045
R squared	0.993
IC50 approx SE (nM)	1.09
50% inhibition (nM)	26.40

The Y-axis label is RFU/min.


Staurosporine IC_{50} Determination at ATP K_m is 26.4 nM

Summary

Assay Validation Results and Progress Curve and Assay Strength at 1 mM ATP

Experiment	Result
Enzyme Titration Linear Range	0.001 - 0.31 nM
Sensor Peptide K_m Value	8.3 µM
ATP K_m Value	27 µM
DMSO Tolerance (highest % recommended)	2
Staurosporine IC50 Determination at ATP Km is	26.4 nM

Progress Curve

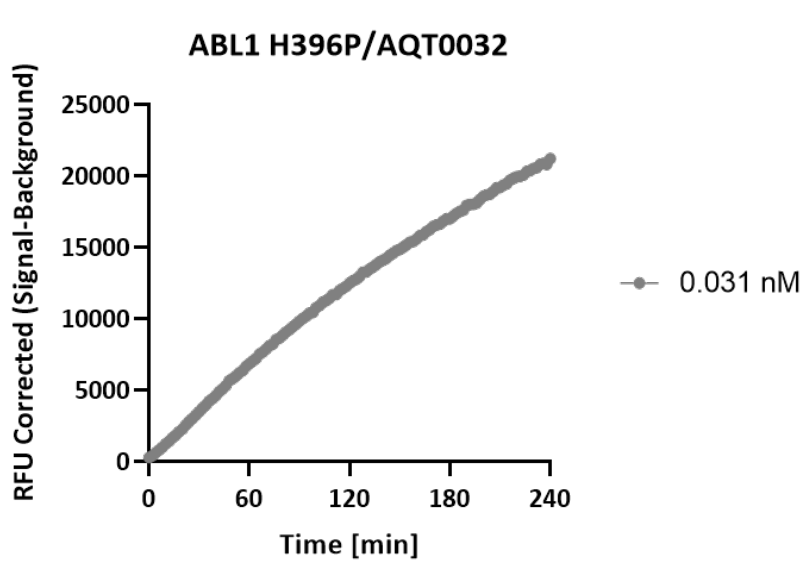

Kinase Name	Conc. (nM)	Sox-based Substrate Name	Normalized Reaction Rate (RFU/pmole/min)	Normalized Rate Stnd Error (RFU/pmole/min)
ABL1 H396P	0.031	AQT0032	181452	734

Assay Strength Key	
Very Strong	>1,000 (RFU/pmole/min)
Strong	300 to 999 (RFU/pmole/min)
Moderate	100 to 299 (RFU/pmole/min)
Weak	30 to 99 (RFU/pmole/min)

Under the conditions utilized for this experiment, the assay is Very Strong