AQT0032 – ABL1 [Y253F] Assay Validation

PhosphoSens®-Kinetic Assay Format

Outline for this Study

PhosphoSens-Kinetic Assay Validation

AssayQuant TECHNOLOGIES INC.

Enzyme Source, Construct, and Lot Information:

SignalChem ABL1 [Y253F] (Cat#/Lot#: A03-12EG/F687-3) amino acids 27-end; N-terminal GST-tag

Reference Compound Information:

Staurosporine MedChem Express

Experiments to be run:

Enzyme Titration

Sensor Peptide K_m Determination

ATP K_m Determination

DMSO Tolerance Test

Reference Compound IC_{50} Determination at ATP K_m

Enzyme Titration

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

15 µM AQT0032

0, 0.00068, 0.002, 0.0061, 0.018, 0.055, 0.16, 0.49, 1.5, 4.4, 13, 40 nM ABL1 [Y253F]

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 or 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:


Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.

Enzyme Titration


Progress Curves


Complete Progress Curves

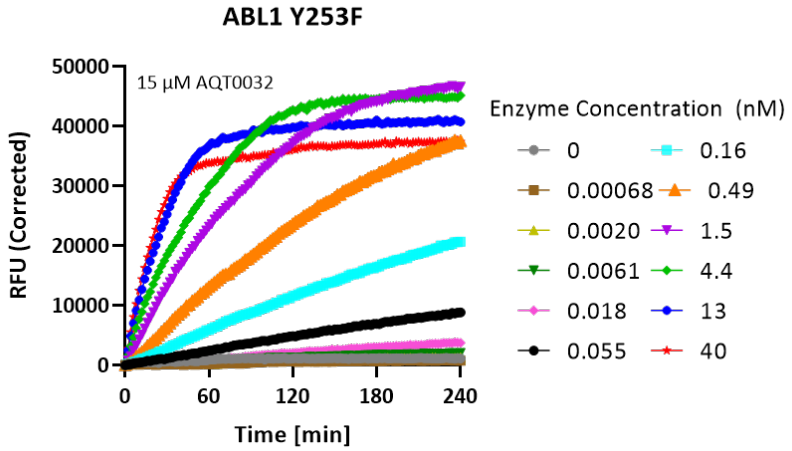

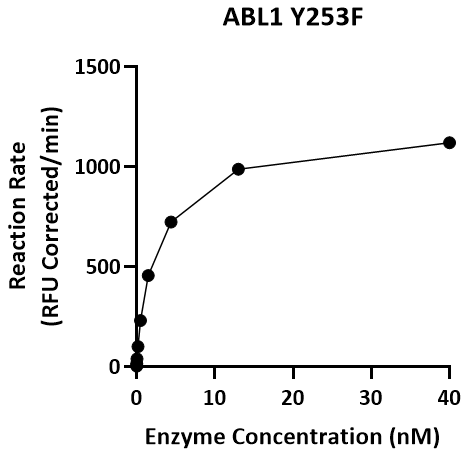

Linear Region of Progress Curves

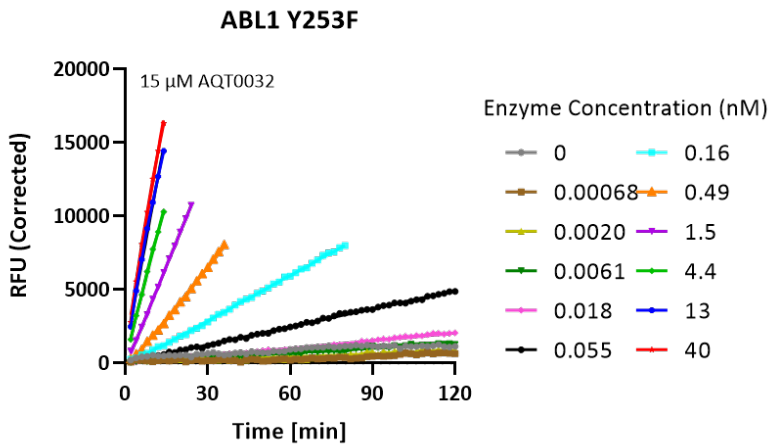

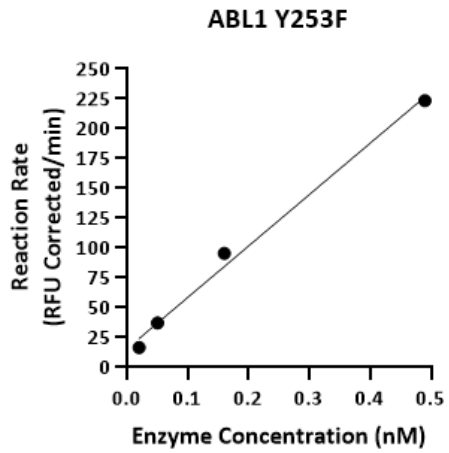

Linear Range

Enzyme Titration

Reaction Rate Table

Enzyme Conc. (nM)	Reaction Rate (RFU/min)	Normalized Reaction Rate (RFU/pmole/min)
0.00068	5	356765
0.002	6	157225
0.0061	10	85410
0.018	17	48000
0.055	41	37036
0.16	102	31969
0.49	231	23612
1.5	457	15247
4.4	724	8232
13	988	3800
40	1121	1401

The reaction is linear from 0.018 - 0.49 nM

Sensor Peptide K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

0, 0.20, 0.39, 0.78, 1.6, 3.1, 6.3, 13, 25, 50, 100, and 200 µM AQT0032

0.16 nM ABL1 [Y253F]

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


Sensor Peptide K_m Determination

Titration Curves and K_m Plot and Table

Sensor Peptide Titration Curves

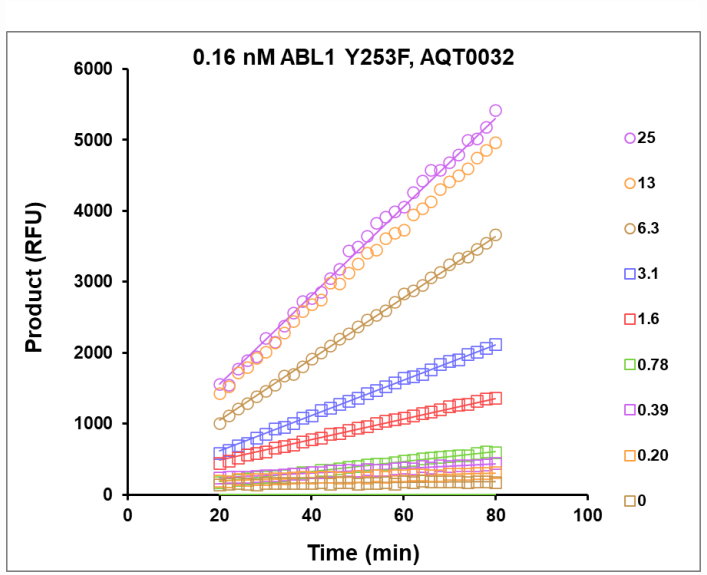

Sensor Peptide K_m Plot

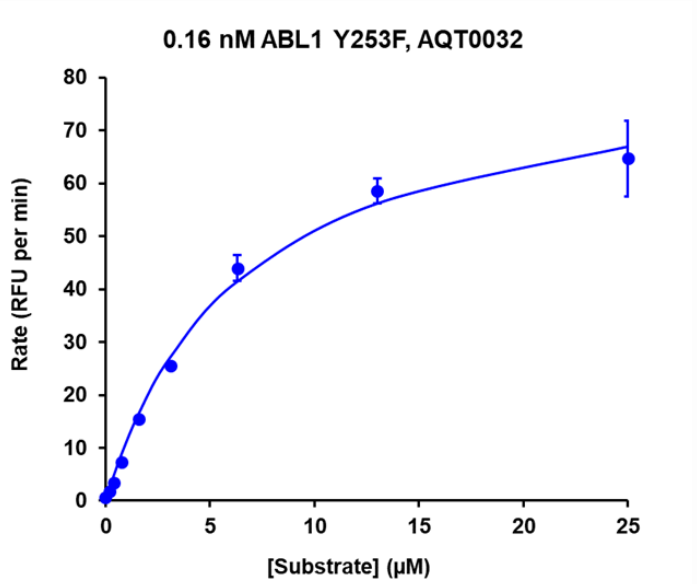

Sensor Peptide K_m Table

Parameter	Value	Approx SE
Vmax (RFU per min)	84.5	2.6
Vmax (RFU per pmol per min)	26399	817
Km (µM)	6.6	0.4
R squared	0.994	

Sensor Peptide K_m is 6.6 µM

ATP K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

0, 2.0, 3.9, 7.8, 16, 31, 63, 125, 250, 500, 1000, and 2000 µM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

15 µM AQT0032

0.16 nM ABL1 [Y253F]

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


ATP K_m Determination

Titration Curves and K_m Plot and Table

ATP Titration Curves

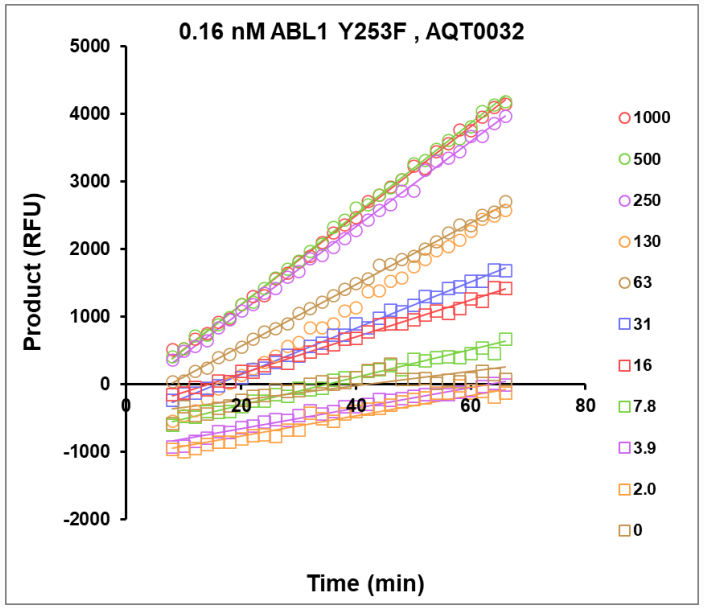

ATP K_m Plot

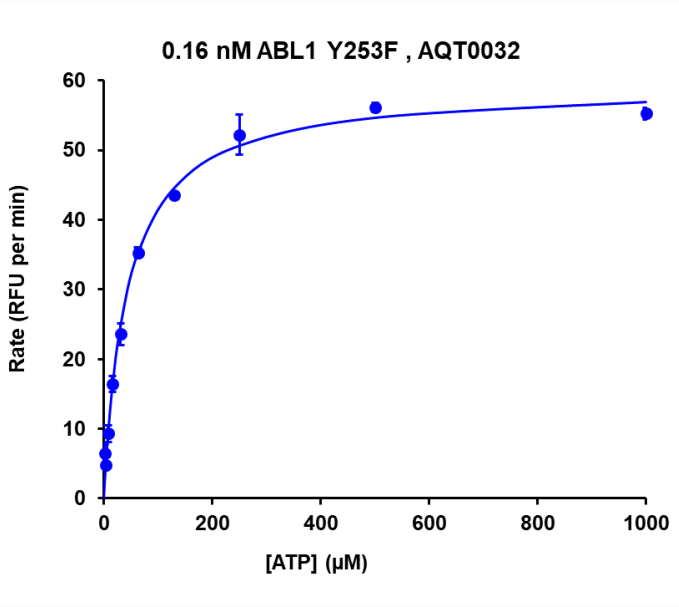

ATP K_m Table

Parameter	Value	Approx SE
Vmax (RFU per min)	59.4	0.5
Vmax (RFU per pmol per min)	18565	157
Km (µM)	43.2	0.3
R squared	0.994	

ATP K_m is 43 µM

DMSO Tolerance Test

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

0, .01, .02, .04, .08, .16, .31, .63, 1.3, 2.5, 5.0, and 10% DMSO

15 µM AQT0032

0.16 nM ABL1 [Y253F]

Reaction Set Up:

2 or 2.5 µL	10x DMSO dilutions
14 or 17.5 µL	Reaction Mix with Sensor Peptide, ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


DMSO Tolerance Test

Titration Curves and Inhibition Plot

Complete Progress Curves

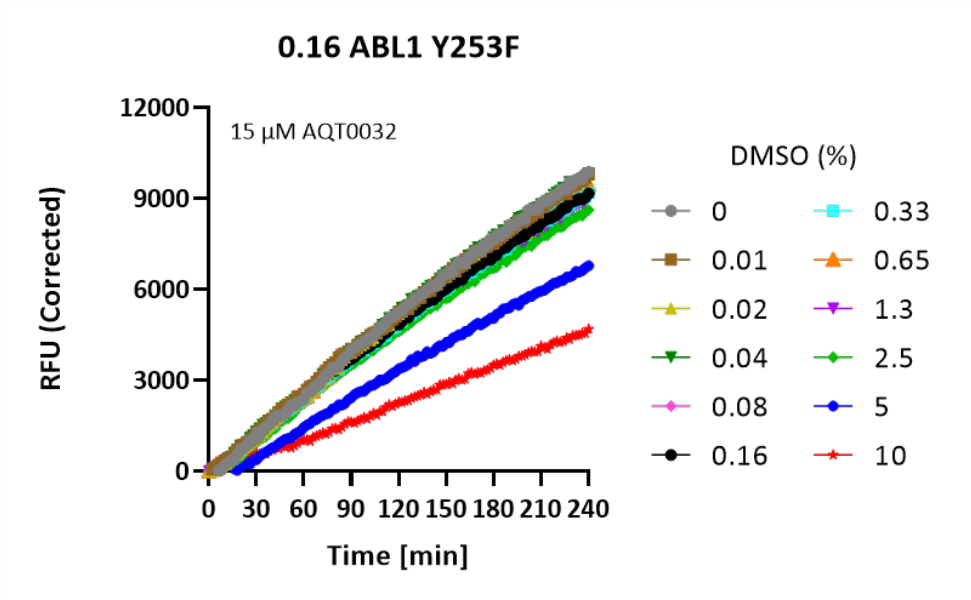

Reaction Rate vs [DMSO] Plot

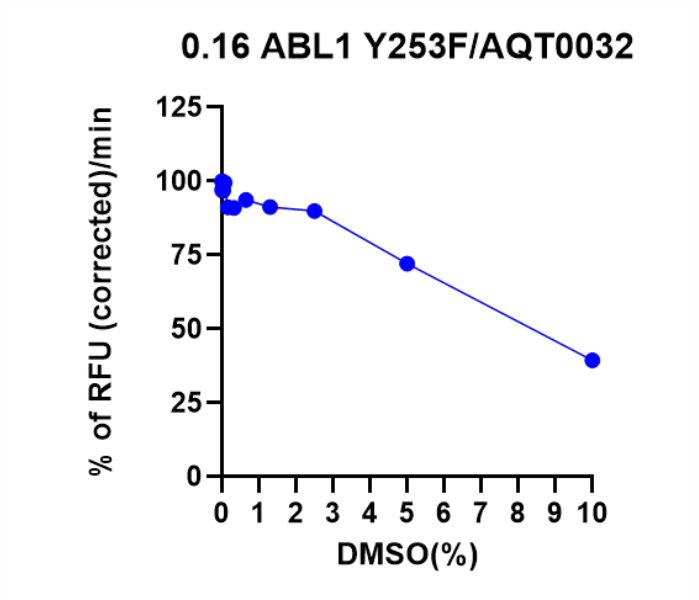

No change in enzyme activity out to 2% DMSO

IC_{50} Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

ATP at K_m

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

2% DMSO

15 µM AQT0032

0.2 nM ABL1 [Y253F]

0, 0.0169, 0.0508, .152, .457, 1.37, 4.12, 12.3, 37, 111, 333, and 1000 nM Staurosporine

Reaction Set Up:

16 µL	Reaction Mix with Sensor Peptide and Inhibitor
4 µL	1x EDB or Kinase dilutions (5x in EDB)
20 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.

Inhibitors are added via direct (0.4 µL of 50X stock in 100% DMSO) or intermediate dilutions (2.0 µL of 10X stock in 10% DMSO).


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


IC_{50} Determination

Progress Curves and IC_{50} Curves and Table


Inhibitor Titration Progress Curves

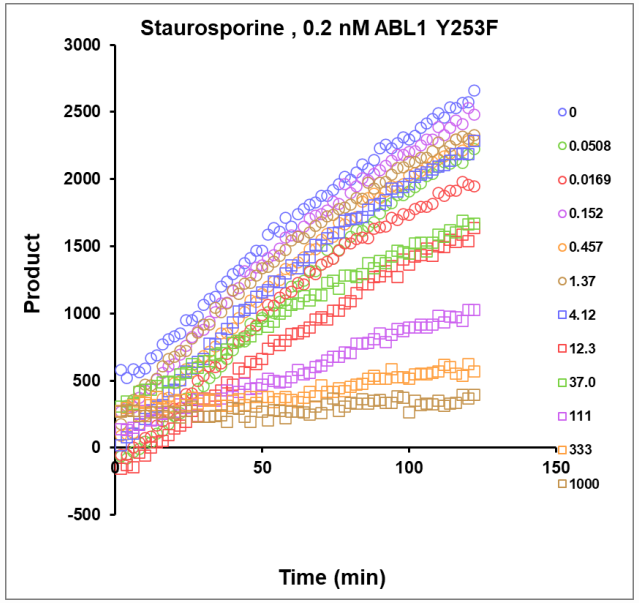

Linear Region of Progress Curves

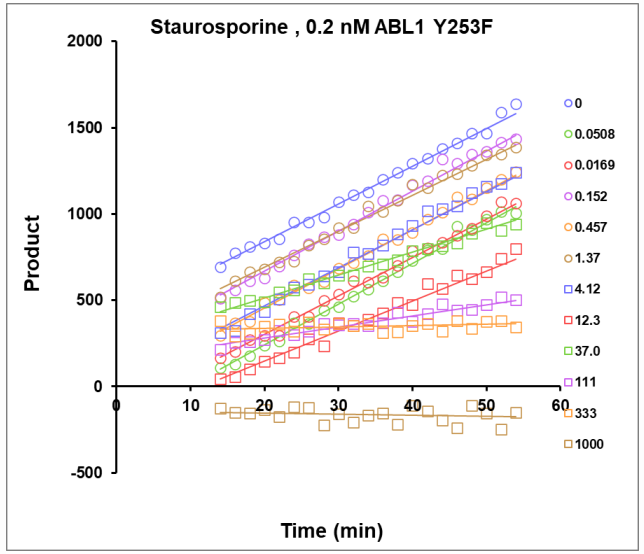

IC_{50} Curve

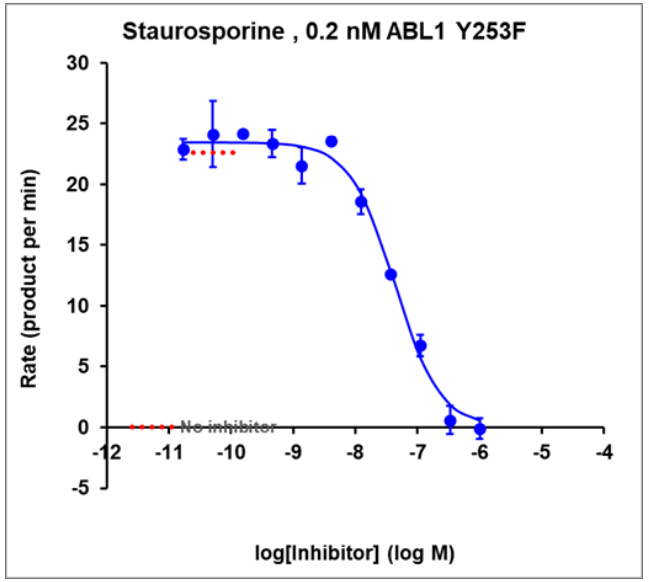

The Y-axis label is RFU/min.

IC_{50} Table

Parameter	Value
Bottom	0.0
Top	23.5
log IC50	-7.37
IC50 (nM)	42.95
Ki (nM)	0.92
Slope	-1.207
R squared	0.990
IC50 approx SE (nM)	0.70
50% inhibition (nM)	42.95


Staurosporine IC_{50} Determination at ATP K_m is 43 nM

Summary

Assay Validation Results and Progress Curve and Assay Strength at 1 mM ATP

Experiment	Result
Enzyme Titration Linear Range	0.018 - 0.49 nM
Sensor Peptide K_m Value	6.6 µM
ATP K_m Value	43 µM
DMSO Tolerance (highest % recommended)	2
Staurosporine IC50 Determination at ATP Km is	43.0 nM

Progress Curve

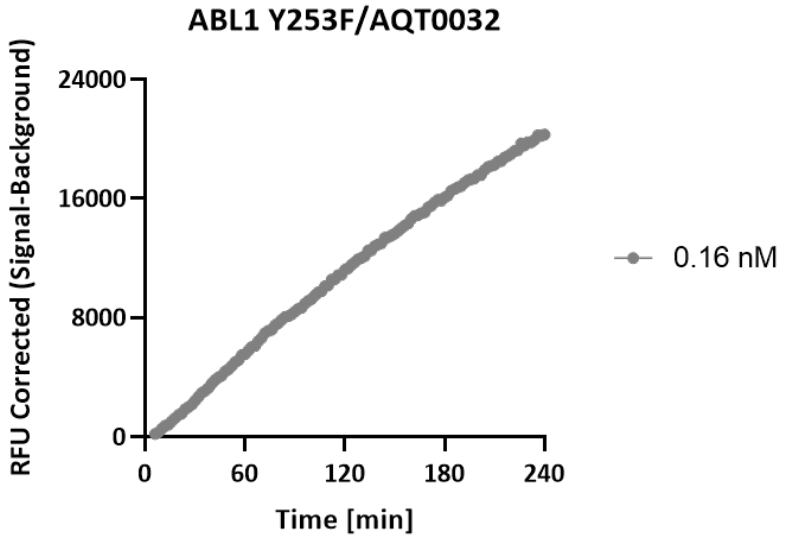

Kinase Name	Conc. (nM)	Sox-based Substrate Name	Normalized Reaction Rate (RFU/pmole/min)	Normalized Rate Stnd Error (RFU/pmole/min)
ABL1 Y253F	0.16	AQT0032	31969	175

Assay Strength Key	
Very Strong	>1,000 (RFU/pmole/min)
Strong	300 to 999 (RFU/pmole/min)
Moderate	100 to 299 (RFU/pmole/min)
Weak	30 to 99 (RFU/pmole/min)

Under the conditions utilized for this experiment, the assay is Very Strong