AQT0260 – DYRK1A Assay Validation

PhosphoSens®-Kinetic Assay Format

Outline for this Study

PhosphoSens-Kinetic Assay Validation

AssayQuant TECHNOLOGIES INC.

Enzyme Source, Construct, and Lot Information:

Carna DYRK1A (Cat/Lot #, 04-130/10CBS-0742Q) amino acids 1-763 (end), N-term GST tag

Reference Compound Information:

Staurosporine MedChem Express

Experiments to be run:

Enzyme Titration

Sensor Peptide K_m Determination

ATP K_m Determination

DMSO Tolerance Test

Reference Compound IC_{50} Determination at ATP K_m

Enzyme Titration

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

20 µM AQT0260

0.01, 0.02, 0.04, 0.08, 0.16, 0.3125, 0.625, 1.25, 2.5, 5, 10 and 20 nM DYRK1A

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 or 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:


Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.

Enzyme Titration


Progress Curves


Complete Progress Curves

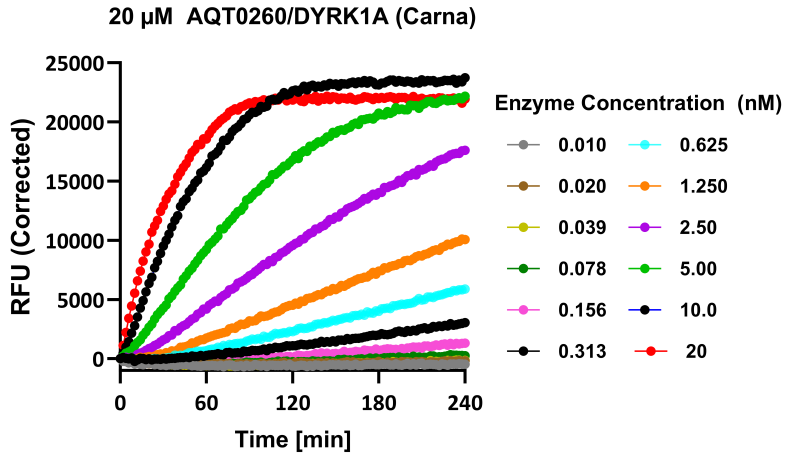

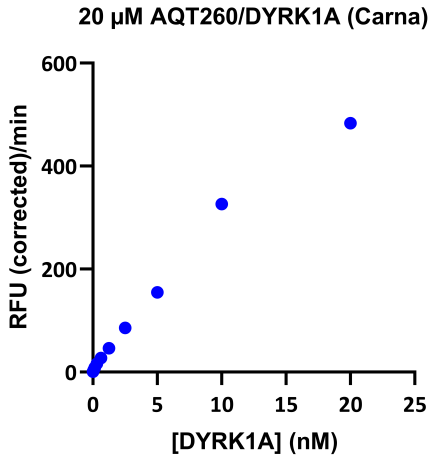

Linear Region of Progress Curves

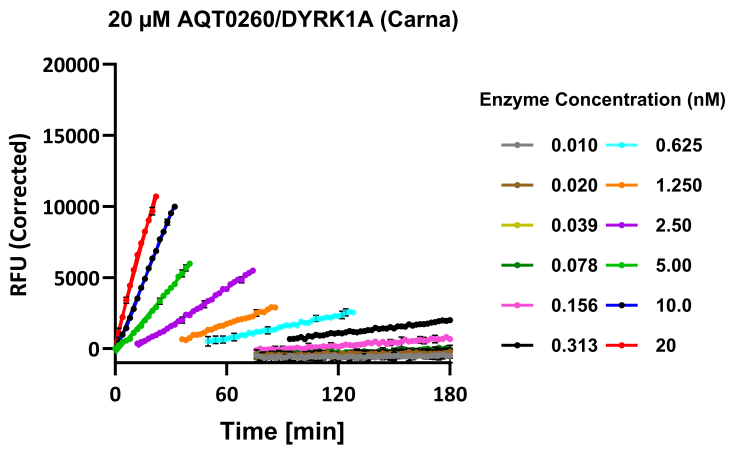

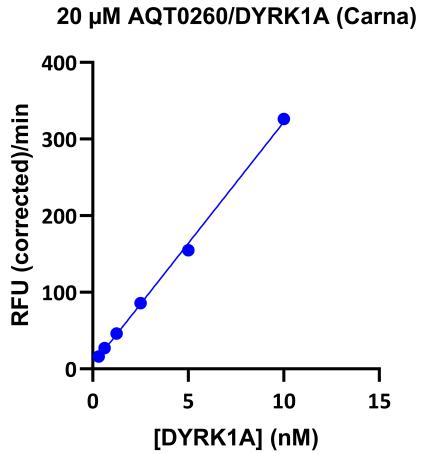

Linear Range

Enzyme Titration

Reaction Rate Table

Enzyme Conc. (nM)	Normalized Reaction Rate (RFU/pmole/ per min)	Normalized Reaction Rate Stnd Error (RFU/pmole/min)
0.01	4753.5	548.5
0.02	3820.0	282.3
0.04	3070.0	151.3
0.08	2712.5	73.2
0.16	*2725.0*	*41.1*
0.33	2424.2	23.5
0.65	*2086.2*	*30.2*
1.3	*1775.8*	*27.2*
2.5	*1717.4*	*19.9*
5	*1547.0*	*29.5*
10	*1630.0*	*17.0*
20	1207.8	30.5

The reaction is linear from 0.65 - 10 nM

Sensor Peptide K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

1, 2, 3, 5, 7, 10, 15, 20, 30, 50, 70, and 100 µM AQT0260

2.5 nM DYRK1A

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


Sensor Peptide K_m Determination

Titration Curves and K_m Plot and Table

Sensor Peptide Titration Curves

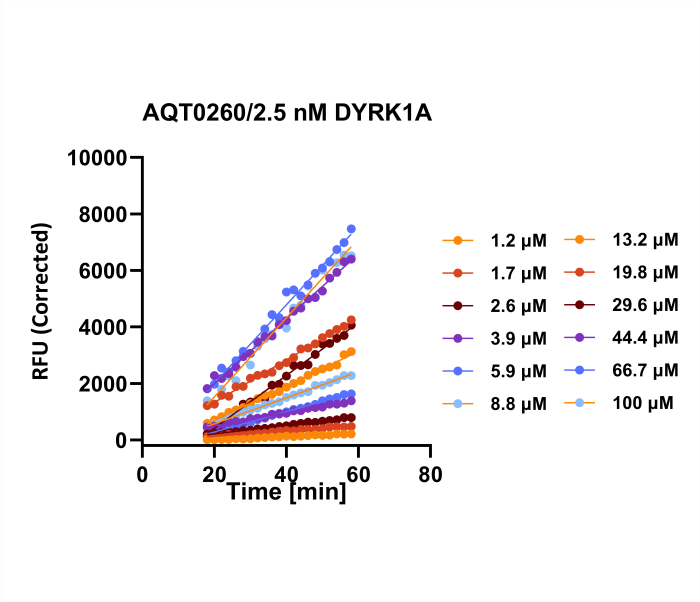

Sensor Peptide K_m Plot

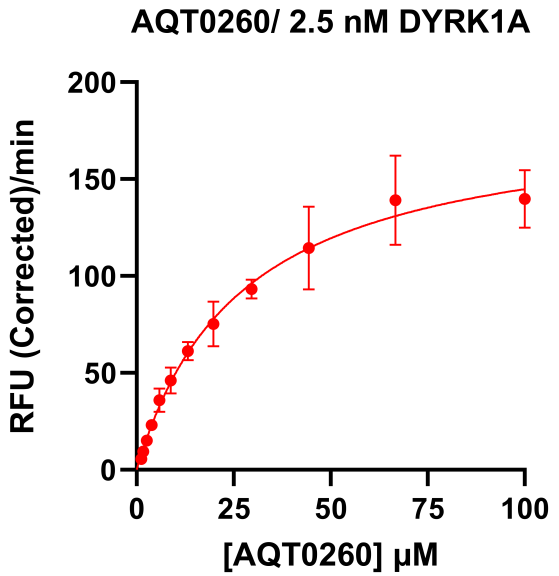

Sensor Peptide K_m Table

Michaelis-Menten	
Best-fit values	
Vmax	183.9
Km	26.99
Std. Error	
Vmax	5.865
Km	2.083
95% CI (asymptotic)	
Vmax	170.8 to 196.9
Km	22.35 to 31.63
Goodness of Fit	
Degrees of Freedom	10
R squared	0.9952
Sum of Squares	126.4
Sy.x	3.556

Sensor Peptide K_m is 27 µM

ATP K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

0, 2.0, 3.9, 7.8, 16, 31, 63, 125, 250, 500, 1000, and 2000 µM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

20 µM AQT0260

2.5 nM DYRK1A

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


ATP K_m Determination

Titration Curves and K_m Plot and Table

ATP Titration Curves

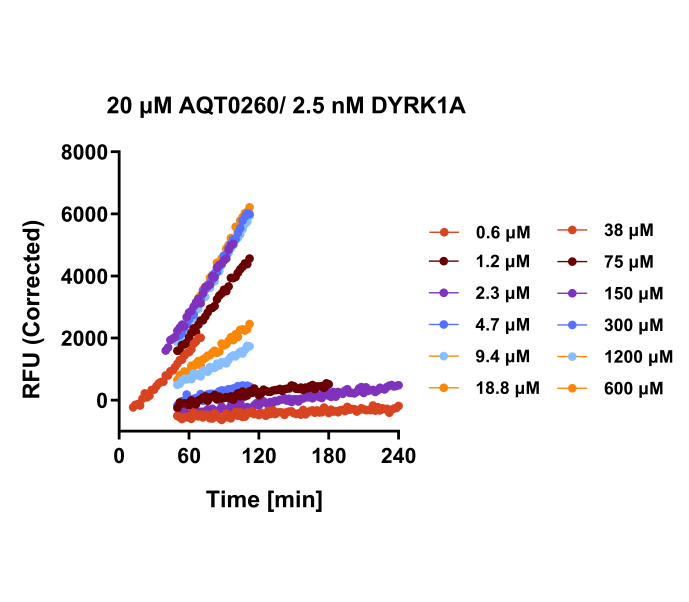

ATP K_m Plot

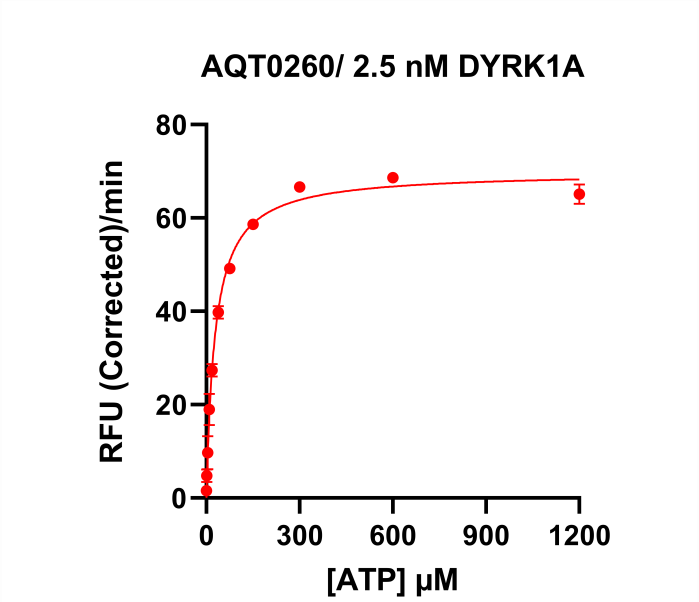

ATP K_m Table

Michaelis-Menten	
Best-fit values	
Vmax	69.87
Km	28.26
Std. Error	
Vmax	1.107
Km	1.942
95% CI (asymptotic)	
Vmax	67.41 to 72.34
Km	23.93 to 32.58
Goodness of Fit	
Degrees of Freedom	10
R squared	0.9961
Sum of Squares	30.40
Sy.x	1.744

ATP K_m is 28 µM

DMSO Tolerance Test

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

0, .01, .02, .04, .08, .16, .31, .63, 1.3, 2.5, 5.0, and 10% DMSO

20 µM AQT0260

2.5 nM DYRK1A

Reaction Set Up:

2 or 2.5 µL	10x DMSO dilutions
14 or 17.5 µL	Reaction Mix with Sensor Peptide, ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


DMSO Tolerance Test

Titration Curves and Inhibition Plot

Complete Progress Curves

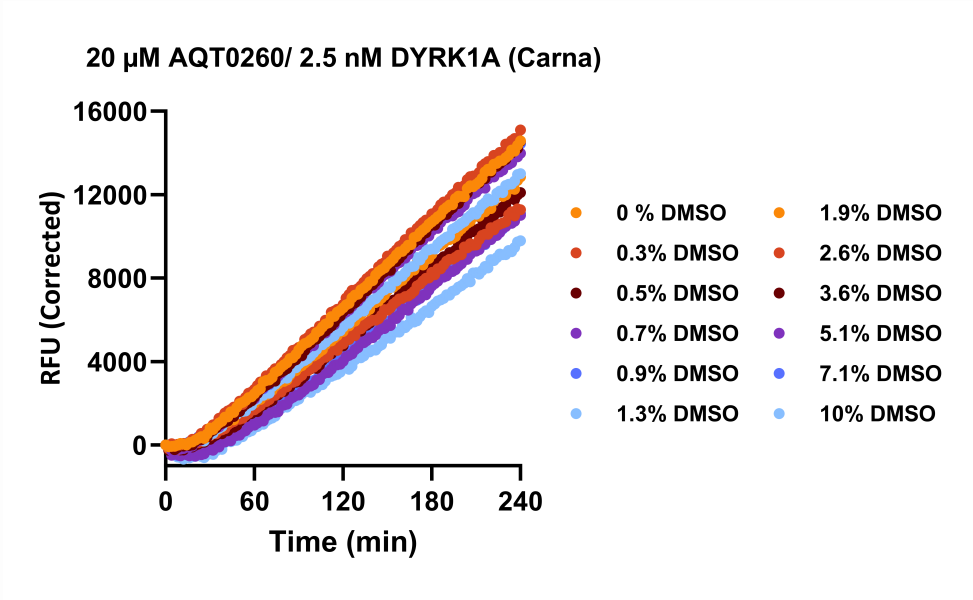

Reaction Rate vs [DMSO] Plot

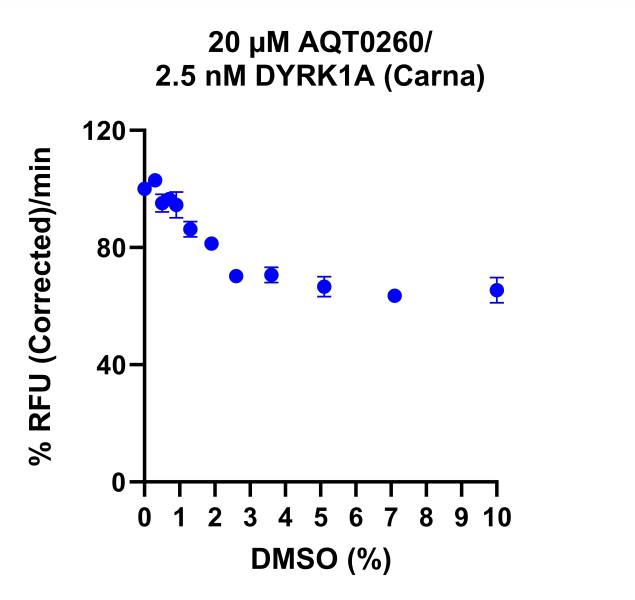

Modest but acceptable decrease in activity up to 2% DMSO

IC_{50} Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

ATP at K_m

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

2% DMSO

20 µM AQT0260

2.5 nM DYRK1A

0, 0.169, 0.508, 1.52, 4.57, 13.7, 41.2, 123, 370, 1110, 3330, 10000 nM Staurosporine

Reaction Set Up:

16 µL	Reaction Mix with Sensor Peptide and Inhibitor
4 µL	1x EDB or Kinase dilutions (5x in EDB)
20 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.

Inhibitors are added via direct (0.4 µL of 50X stock in 100% DMSO) or intermediate dilutions (2.0 µL of 10X stock in 10% DMSO).


Notes:

Enzyme Dilution Buffer (EDB):20 mM HEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


IC_{50} Determination

Progress Curves and IC_{50} Curves and Table


Inhibitor Titration Progress Curves

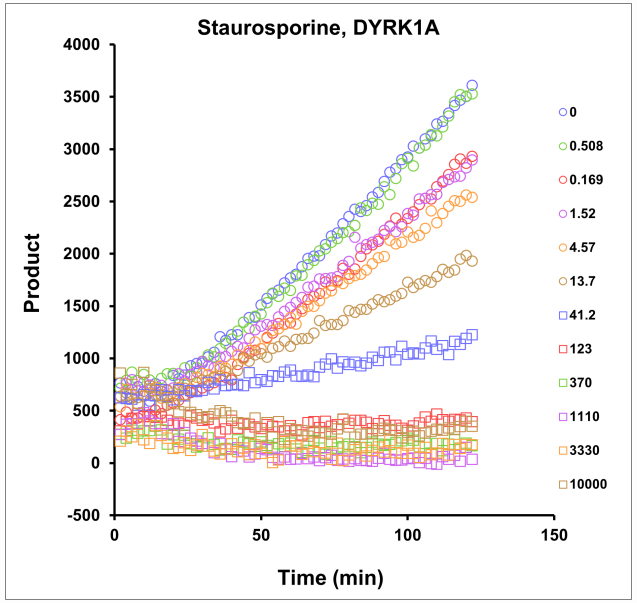

Linear Region of Progress Curves

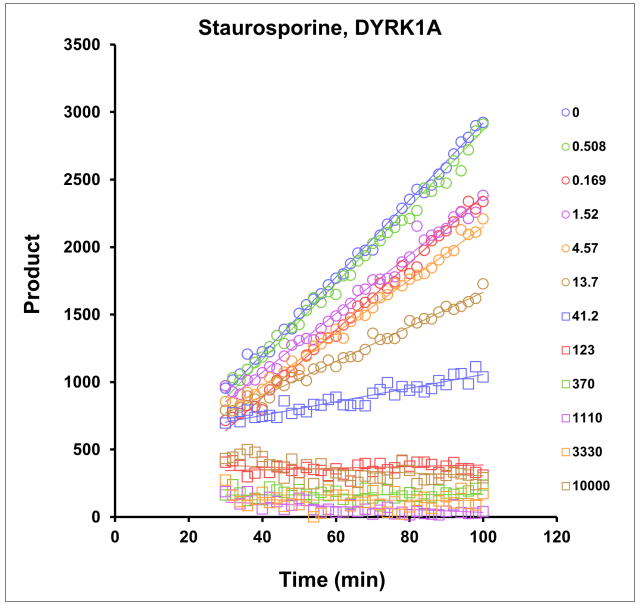

IC_{50} Curve

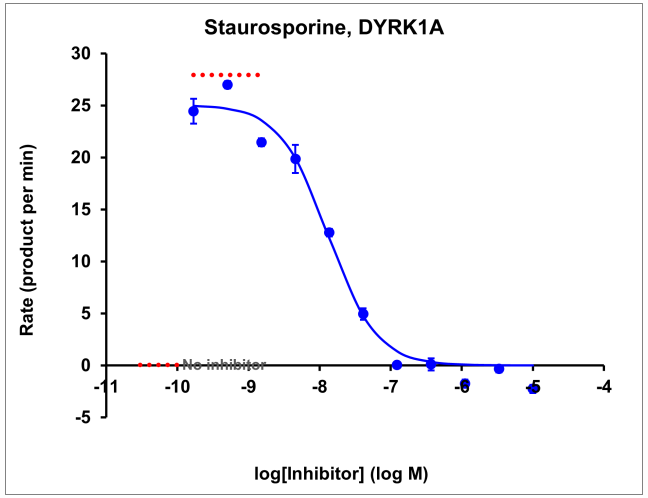

IC_{50} Table

Parameter	Value
Bottom	0.0
Top	25.1
log IC50	-7.88
IC50 (nM)	13.18
Ki (nM)	6.59
Slope	-1.278
R squared	0.985
IC50 approx SE (nM)	0.32
50% inhibition (nM)	13.18

The Y-axis label is RFU/min.


Staurosporine IC_{50} Determination at ATP K_m is 13 nM

Summary

Assay Validation Results and Progress Curve and Assay Strength at 1 mM ATP

Experiment	Result
Enzyme Titration Linear Range	0.65 - 10 nM
Sensor Peptide K_m Value	27 µM
ATP K_m Value	28 µM
DMSO Tolerance (highest % recommended)	2
Staurosporine IC_{50} Determination at ATP K_m	13 nM

Progress Curve

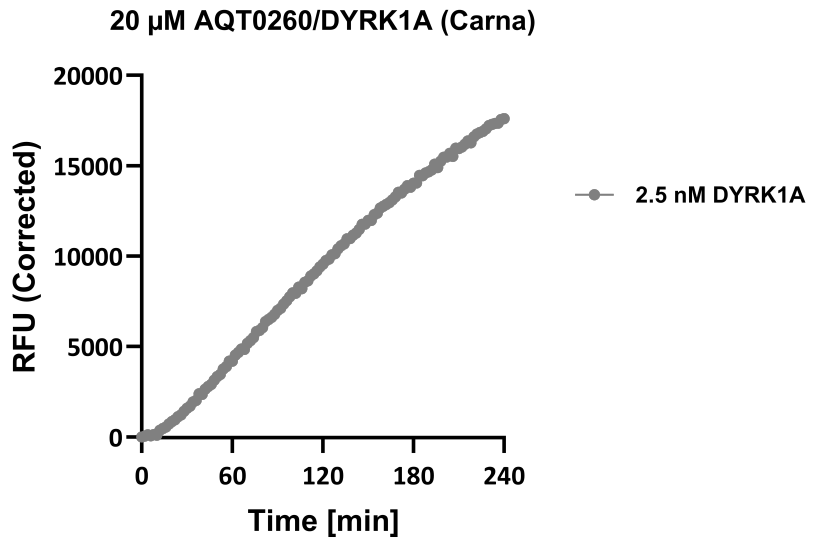

Kinase Name	Conc. (nM)	Sox-based substrate name	Normalized Reaction Rate (RFU/pmol/min)	Normalized Reaction Rate Stnd Error (RFU/pmol/min)
DYRK1A	2.5	AQT0260	1717	27

Assay Strength Key	
Very Strong	>1,000 (RFU/pmole/min)
Strong	300 to 999 (RFU/pmole/min)
Moderate	100 to 299 (RFU/pmole/min)
Weak	30 to 99 (RFU/pmole/min)

Under the conditions utilized for this experiment, the assay is Very Strong