AQT0260 – DYRK1B Assay Validation

PhosphoSens®-Kinetic Assay Format

Outline for this Study

PhosphoSens-Kinetic Assay Validation

AssayQuant TECHNOLOGIES INC.

Enzyme Source, Construct, and Lot Information:

Carna DYRK1A (Cat/Lot #, 04-131/21CBS-0511B) amino acids 1-629 (end), N-term GST tag

Reference Compound Information:

Staurosporine MedChem Express

Experiments to be run:

Enzyme Titration

Sensor Peptide K_m Determination

ATP K_m Determination

DMSO Tolerance Test

Reference Compound IC_{50} Determination at ATP K_m

Enzyme Titration

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

20 µM AQT0260

0.01, 0.02, 0.04, 0.08, 0.16, 0.3125, 0.625, 1.25, 2.5, 5, 10 and 20 nM DYRK1B

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 or 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.

Notes:


Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


Enzyme Titration

Progress Curves


AssayQuant TECHNOLOGIES INC.


Complete Progress Curves

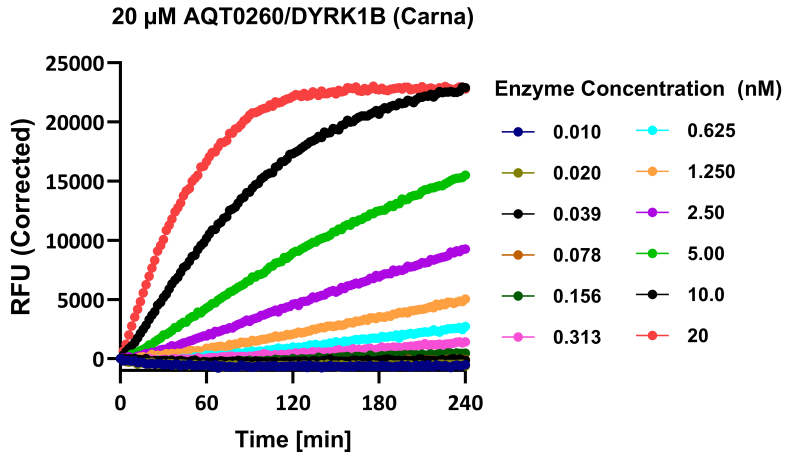

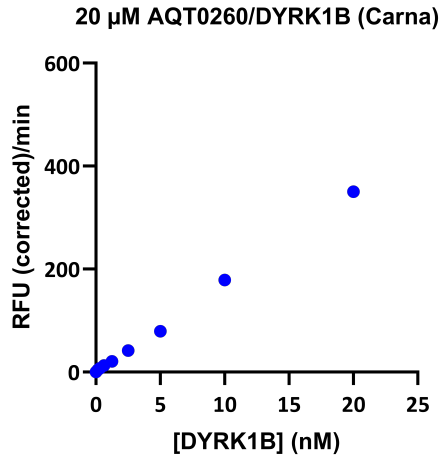

Linear Region of Progress Curves

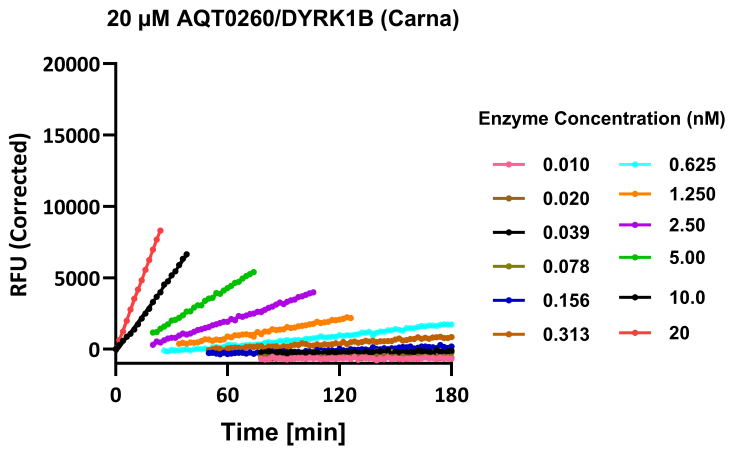

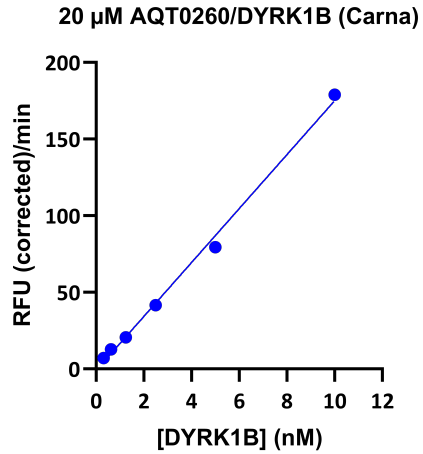

Linear Range

Enzyme Titration

Reaction Rate Table

Enzyme Conc. (nM)	Normalized Reaction Rate (RFU/pmole/ per min)	Normalized Reaction Rate Stnd Error (RFU/pmole/min)
0.01	1583.5	611.5
0.02	1594.5	691.5
0.04	1488.8	328.5
0.08	1343.1	100.6
0.16	*1336.3*	*37.7*
0.33	1084.5	53.7
0.65	*985.4*	*26.4*
1.3	*789.2*	*24.3*
2.5	*832.0*	*7.9*
5	*794.0*	*12.4*
10	*894.5*	*10.2*
20	875.5	5.1

The reaction is linear from 0.65 - 10 nM

Sensor Peptide K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

1, 2, 3, 5, 7, 10, 15, 20, 30, 50, 70, and 100 µM AQT0260

3.0 nM DYRK1B

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mM HEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


Sensor Peptide K_m Determination

Titration Curves and K_m Plot and Table

Sensor Peptide Titration Curves

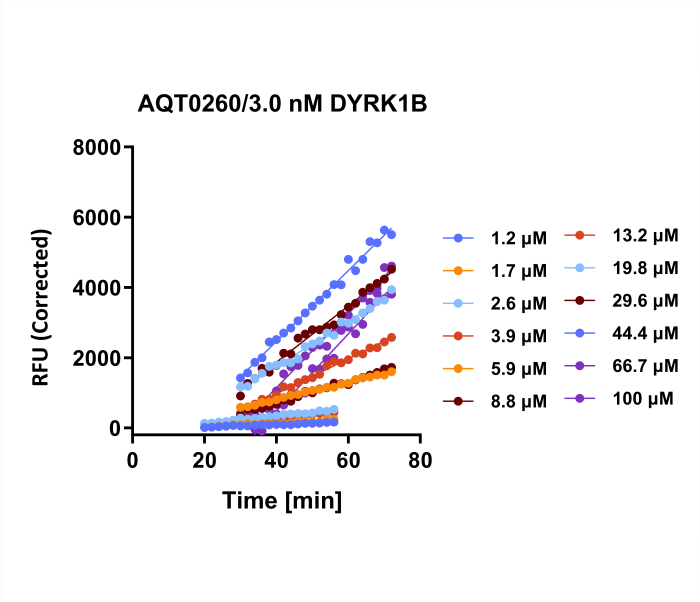

Sensor Peptide K_m Plot

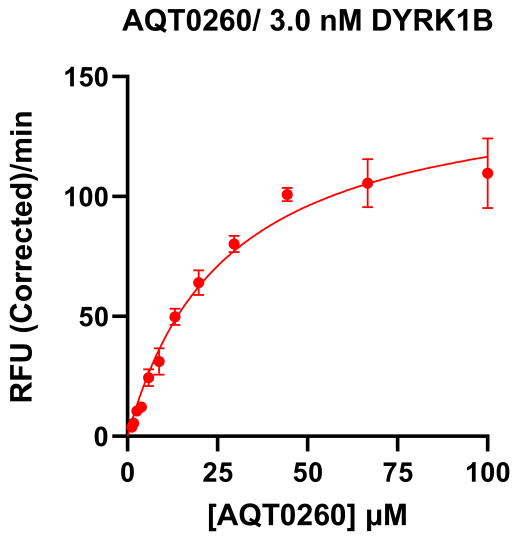

Sensor Peptide K_m Table

Michaelis-Menten	
Best-fit values	
Vmax	148.3
Km	27.23
Std. Error	
Vmax	8.009
Km	3.548
95% CI (asymptotic)	
Vmax	130.4 to 166.1
Km	19.32 to 35.13
Goodness of Fit	
Degrees of Freedom	10
R squared	0.9874
Sum of Squares	232.5
Sy.x	4.822

Sensor Peptide K_m is 27 µM

ATP K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

0, 2.0, 3.9, 7.8, 16, 31, 63, 125, 250, 500, 1000, and 2000 µM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

20 µM AQT0260

3.0 nM DYRK1B

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mM HEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


ATP K_m Determination

Titration Curves and K_m Plot and Table

ATP Titration Curves

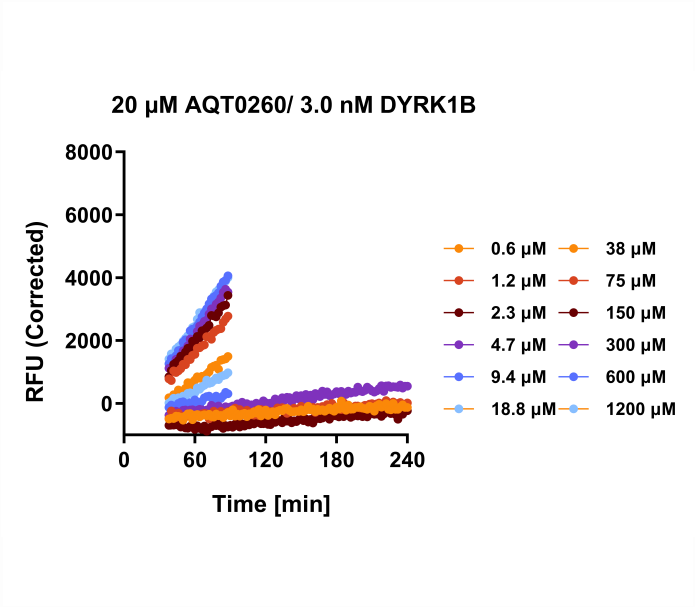

ATP K_m Plot

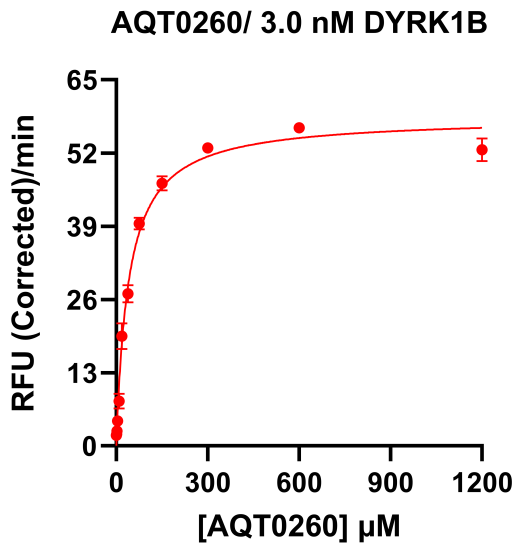

ATP K_m Table

Michaelis-Menten	
Best-fit values	
Vmax	58.37
Km	40.88
Std. Error	
Vmax	1.391
Km	3.977
95% CI (asymptotic)	
Vmax	55.27 to 61.47
Km	32.02 to 49.74
Goodness of Fit	
Degrees of Freedom	10
R squared	0.9929
Sum of Squares	39.18
Sy.x	1.979

ATP K_m is 41 µM

DMSO Tolerance Test

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

0, .01, .02, .04, .08, .16, .31, .63, 1.3, 2.5, 5.0, and 10% DMSO

20 µM AQT0260

3.0 nM DYRK1B

Reaction Set Up:

2 or 2.5 µL	10x DMSO dilutions
14 or 17.5 µL	Reaction Mix with Sensor Peptide, ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 m MHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


DMSO Tolerance Test

Titration Curves and Inhibition Plot

Complete Progress Curves

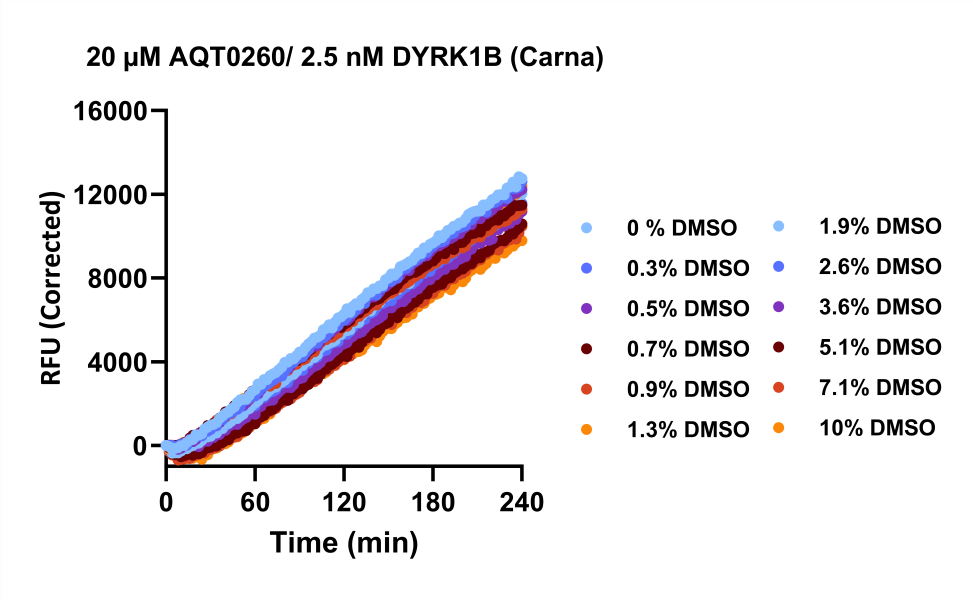

Reaction Rate vs [DMSO] Plot

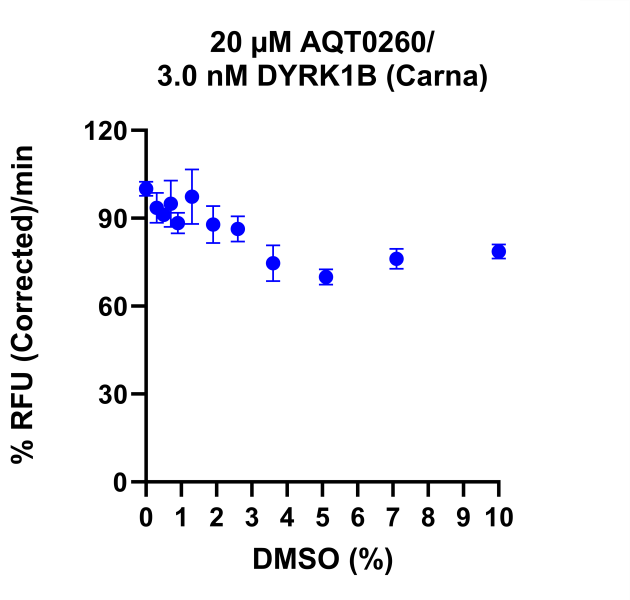

Modest but acceptable decrease in activity up to 2% DMSO

IC_{50} Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

ATP at K_m

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

2% DMSO

20 µM AQT0260

3.0 nM DYRK1B

0, 0.169, 0.508, 1.52, 4.57, 13.7, 41.2, 123, 370, 1110, 3330, 10000 nM Staurosporine

Reaction Set Up:

16 µL	Reaction Mix with Sensor Peptide and Inhibitor
4 µL	1x EDB or Kinase dilutions (5x in EDB)
20 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.

Inhibitors are added via direct (0.4 µL of 50X stock in 100% DMSO) or intermediate dilutions (2.0 µL of 10X stock in 10% DMSO).


Notes:

Enzyme Dilution Buffer (EDB):20 mM HEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine Serum Albumin.


IC_{50} Determination

Progress Curves and IC_{50} Curves and Table


Inhibitor Titration Progress Curves

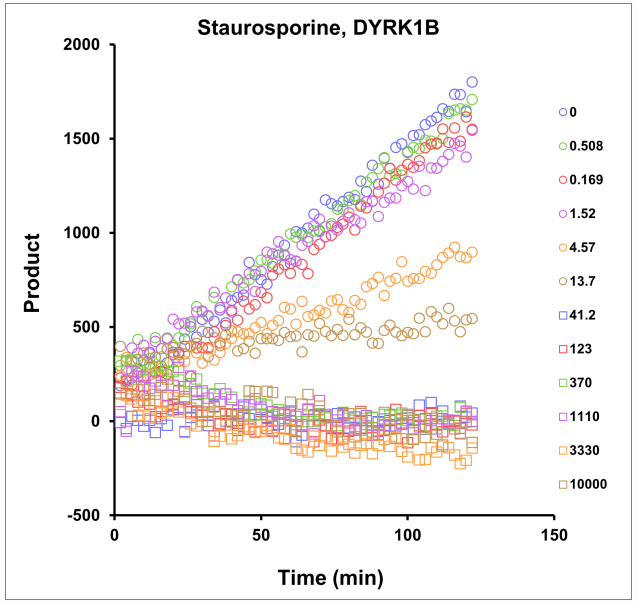

Linear Region of Progress Curves

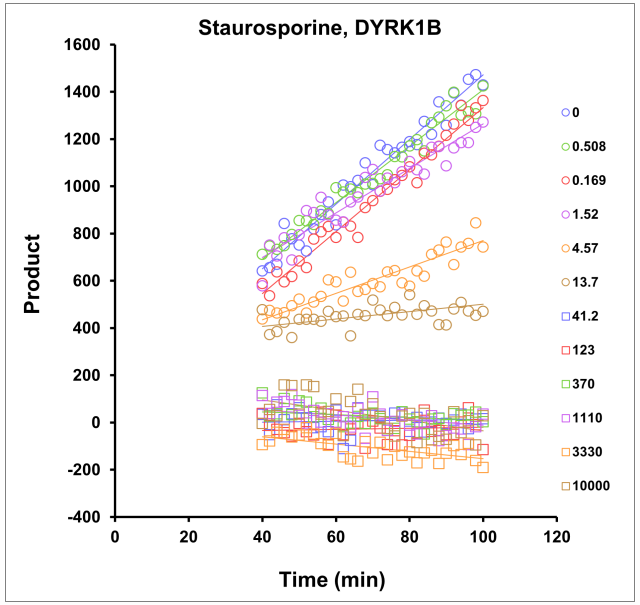

IC_{50} Curve

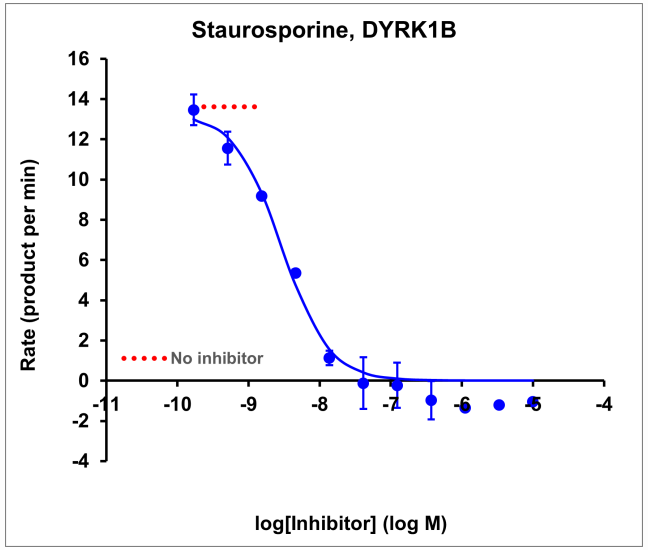

The Y-axis label is RFU/min.

IC_{50} Table

Paramete	Value
Bottom	0.0
Top	13.3
log IC50	-8.53
IC50 (nM)	2.93
Ki (nM)	1.47
Slope	-1.311
R squared	0.978
IC50 approx SE (nM)	0.00
50% inhibition (nM)	2.93


Staurosporine IC_{50} Determination at ATP K_m is 3 nM

Summary

Assay Validation Results and Progress Curve and Assay Strength at 1 mM ATP

Experiment	Result
Enzyme Titration Linear Range	0.65 - 10 nM
Sensor Peptide K_m Value	27 µM
ATP K_m Value	41 µM
DMSO Tolerance (highest % recommended)	2
Staurosporine IC_{50} Determination at ATP K_m	3 nM

Progress Curve

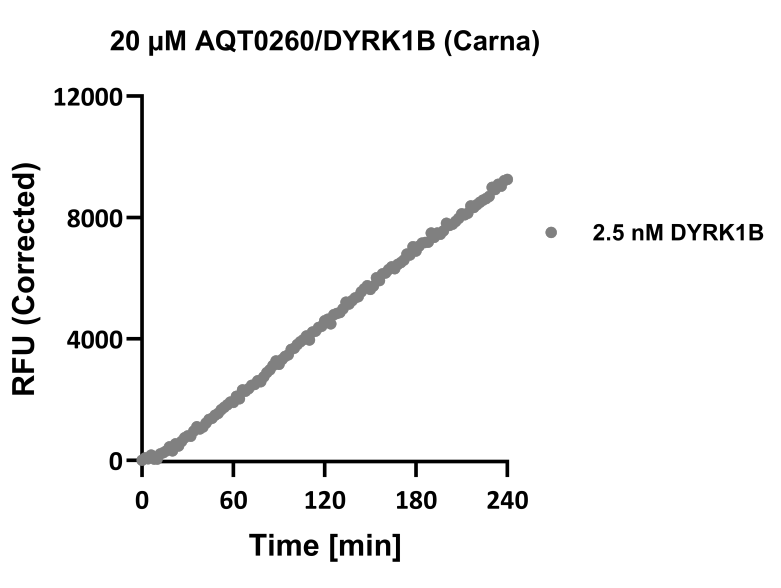

ase Name	Conc. (nM)	Sox-based substrate name	Normalized Reaction Rate (RFU/pmol/min)	Normalized Reaction Rate Stnd Error (RFU/pmol/min)
DYRK1B	2.5	AQT0260	832	8

Assay Strength Key	
Very Strong	>1,000 (RFU/pmole/min)
Strong	300 to 999 (RFU/pmole/min)
Moderate	100 to 299 (RFU/pmole/min)
Weak	30 to 99 (RFU/pmole/min)

Under the conditions utilized for this experiment, the assay is Strong