AQT0297 – CDK2/CycE1 Assay Validation

PhosphoSens®-Kinetic Assay Format

Outline for this Study

PhosphoSens-Kinetic Assay Validation

AssayQuant TECHNOLOGIES INC.

Enzyme Source, Construct, and Lot Information:

Carna CDK2/CycE1 (Cat/Lot #, 04-165/20CBS-0731S) amino acids full length, N-term GST tag & full length CyclinE1

Reference Compound Information:

Staurosporine

Experiments to be run:

Enzyme Titration

Sensor Peptide K_m Determination

ATP K_m Determination

DMSO Tolerance Test

Reference Compound IC_{50} Determination at ATP K_m

Enzyme Titration

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

15µM AQT0297

0.005, 0.01, 0.02, 0.04, 0.08, 0.16, 0.3125, 0.625, 1.25, 2.5, 5 and 10 nM CDK2/CycE1

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 or 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:


Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.

Enzyme Titration


Progress Curves


Complete Progress Curves

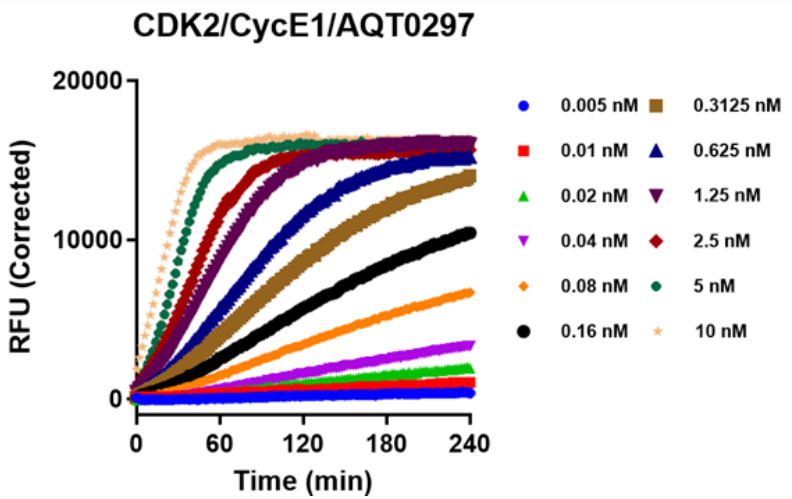

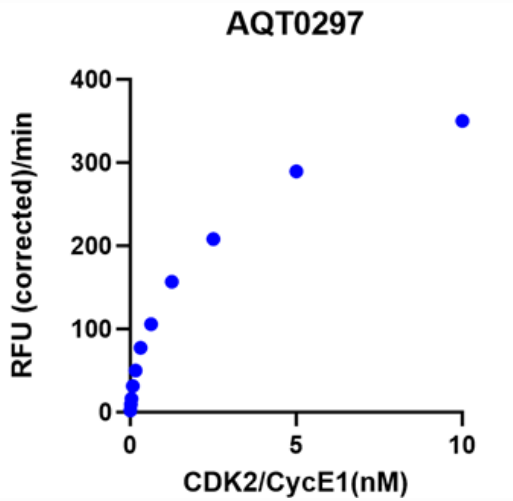

Linear Region of Progress Curves

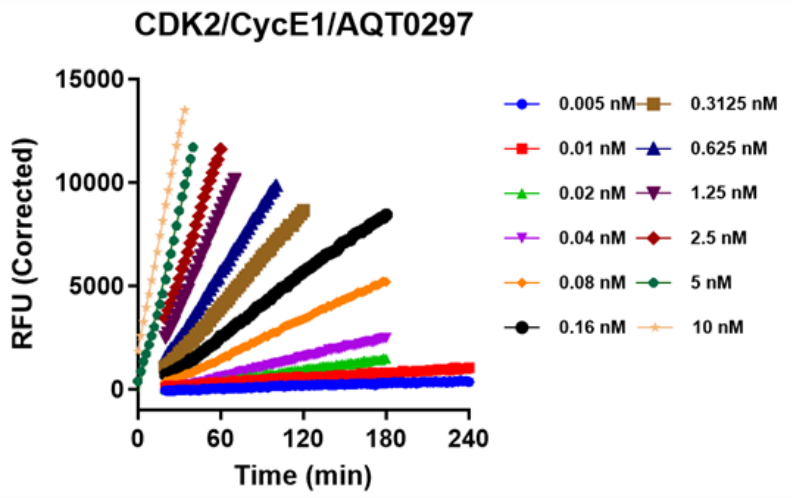

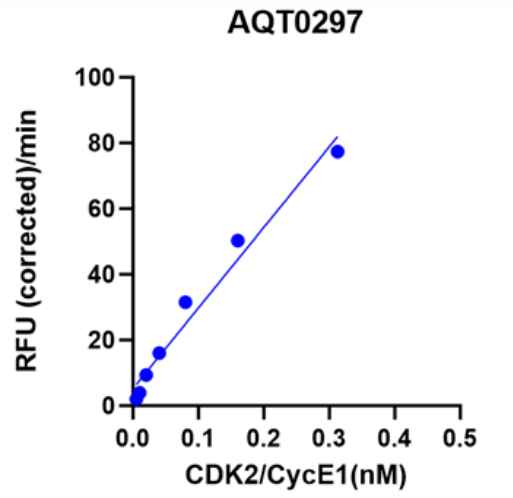

Linear Range

Enzyme Titration

Reaction Rate Table

Enzyme Conc. (nM)	Normalized Reaction Rate (RFU/pmole/min)	Normalized Rate Stnd Error (RFU/pmole/min)
0.005	20,780	355
0.01	19,850	207
0.02	47,075	296
0.04	40,075	174
0.08	39,388	123
0.16	31,419	115
0.3125	24,191	82
0.625	16,928	56
1.25	12,536	53
2.5	8,328	52
5	5,790	110
10	3,500	22

The reaction is linear from 0.04 - 0.31 nM

Sensor Peptide K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

1, 2, 3, 5, 7, 10, 15, 20, 30, 50, 70, & 100µM AQT0297

0.5 nM CDK2/CycE1

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


Sensor Peptide K_m Determination

Titration Curves and K_m Plot and Table

Sensor Peptide Titration Curves

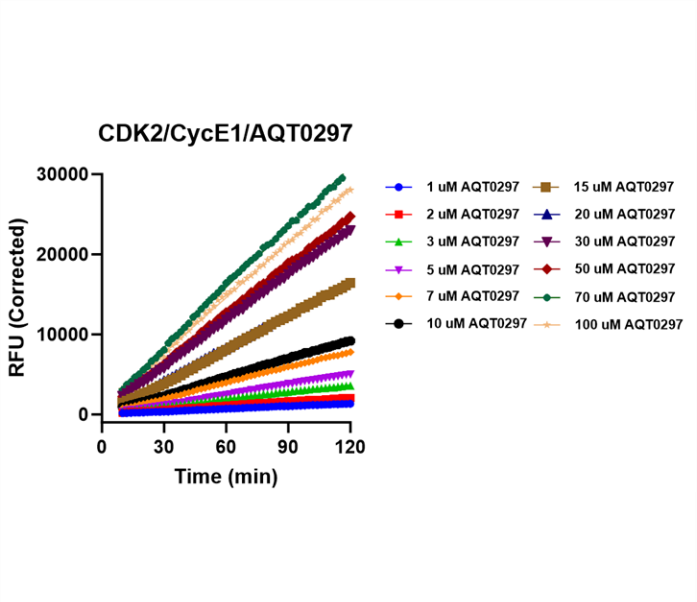

Sensor Peptide K_m Plot

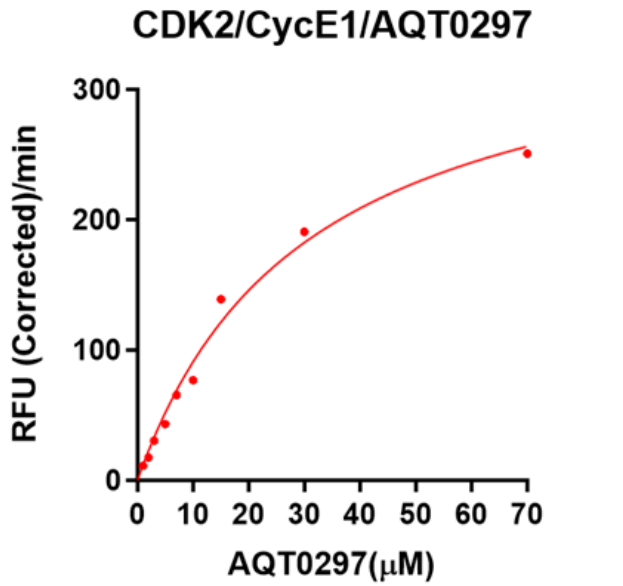

Sensor Peptide K_m Table

Michaelis-Menten	
Best-fit values	
Vmax	367.4
Km	30.41
Std. Error	
Vmax	27.88
Km	4.645
95% CI (profile likelihood)	
Vmax	311.6 to 442.5
Km	21.72 to 43.68
Goodness of Fit	
Degrees of Freedom	7
R squared	0.9872

Sensor Peptide K_m is 30 μM

ATP K_m Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

0, 2.0, 3.9, 7.8, 16, 31, 63, 125, 250, 500, 1000, and 2000 µM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

15µM AQT0297

0.5 nM CDK2/CycE1

Reaction Set Up:

2 or 2.5 µL	10x Sensor Peptide
14 or 17.5 µL	Reaction Mix with ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


ATP K_m Determination

Titration Curves and K_m Plot and Table

ATP Titration Curves

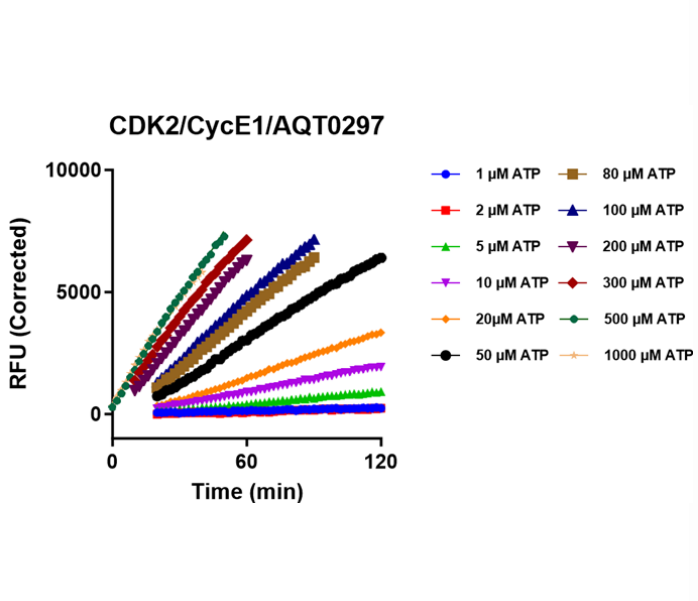

ATP K_m Plot

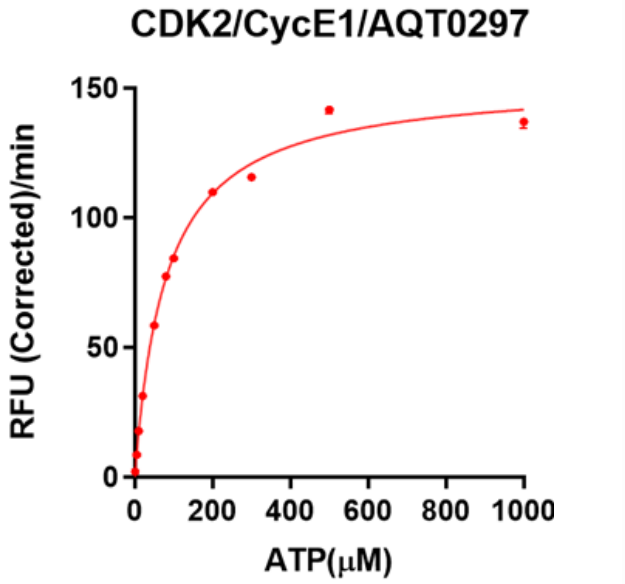

ATP K_m Table

Michaelis-Menten	
Best-fit values	
Vmax	152.9
Km	79.64
Std. Error	
Vmax	3.552
Km	6.255
95% CI (profile likelihood)	
Vmax	145.2 to 161.0
Km	66.76 to 94.71
Goodness of Fit	
Degrees of Freedom	10
R squared	0.9951

ATP K_m is 80 µM

DMSO Tolerance Test

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

1 mM ATP

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

0, .01, .02, .04, .08, .16, .31, .63, 1.3, 2.5, 5.0, and 10% DMSO

15µM AQT0297

0.5 nM CDK2/CycE1

Reaction Set Up:

2 or 2.5 µL	10x DMSO dilutions
14 or 17.5 µL	Reaction Mix with Sensor Peptide, ATP & DTT
4 or 5 µL	1x EDB or Kinase dilutions (5x in EDB)
20 or 25 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 25 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


DMSO Tolerance Test

Titration Curves and Inhibition Plot

Complete Progress Curves

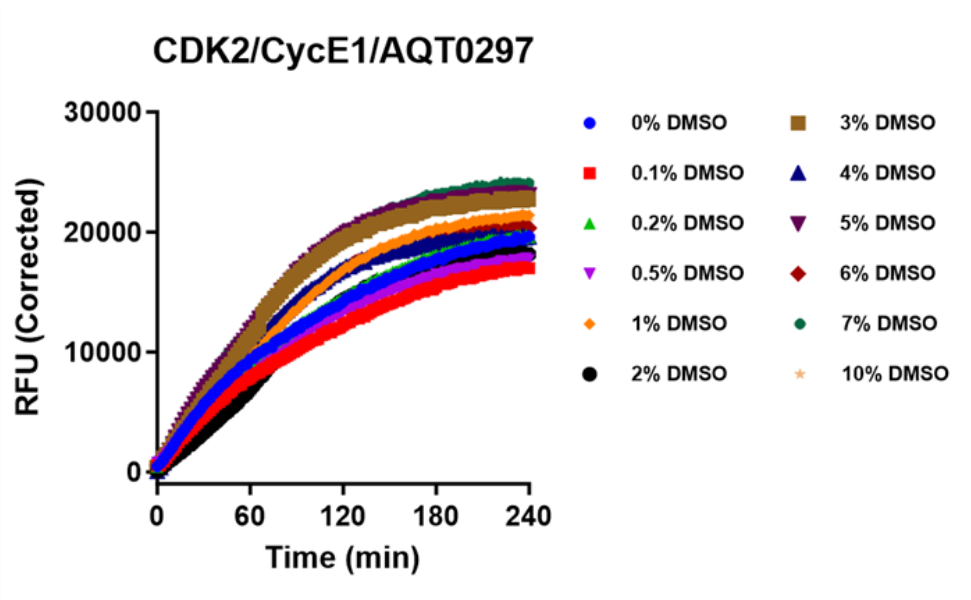

Reaction Rate vs [DMSO] Plot

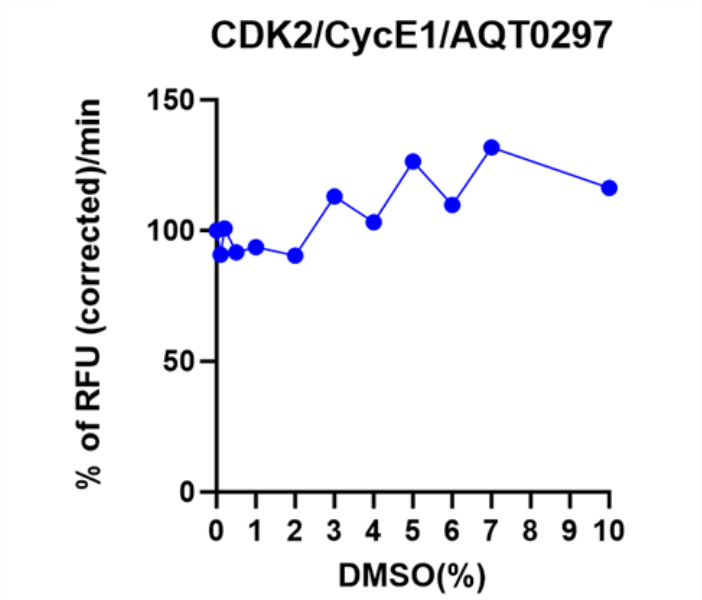

No change in enzyme activity out to 2% DMSO

IC_{50} Determination

Reaction Conditions and Set Up

Reaction Conditions:

54 mM HEPES, pH 7.5

ATP at K_m

1.2 mM DTT

0.012% Brij-35

1% glycerol

0.2 mg/ml BSA

0.55 mM EGTA

10 mM $MgCl_2$

1% DMSO

15µM AQT0297

0.5 nM CDK2/CycE1

0.1 mM Staurosporine with 3-fold titration in 100% DMSO then diluted 10-fold into BSA (with a final concentration of 0.2 mg/ml) for a DMSO concentration of 10% before diluted 10-fold into reaction mixture with a final DMSO concentration of 1%

Reaction Set Up:

16 µL	Reaction Mix with Sensor Peptide and Inhibitor
4 µL	1x EDB or Kinase dilutions (5x in EDB)
20 µL	Final reaction volume

Reactions were run at 30˚C for 240 minutes in either Corning, low volume 384-well, white flat round bottom polystyrene NBS microplates (Cat. #3824) at 20 µL final well volume or in in PerkinElmer, ProxiPlate-384 Plus, white shallow well microplates (Cat. #6008280) at 20 µL final well volumeafter sealing using optically-clear adhesive film (TopSealA-Plus plate seal, PerkinElmer [Cat. #6050185]) in a Biotek Synergy Neo 2 microplate reader with excitation (360 nm) and emission (485 nm) wavelengths.

Inhibitors are added via direct (0.4 µL of 50X stock in 100% DMSO) or intermediate dilutions (2.0 µL of 10X stock in 10% DMSO).


Notes:

Enzyme Dilution Buffer (EDB):20 mMHEPES, pH 7.5,0.01% Brij-35, 5% Glycerol, 0.5 mM EGTA, 1 mM DTT, 1 mg/ml Bovine SerumAlbumin.


IC_{50} Determination

Progress Curves and IC_{50} Curves and Table

Linear Region of Progress Curves

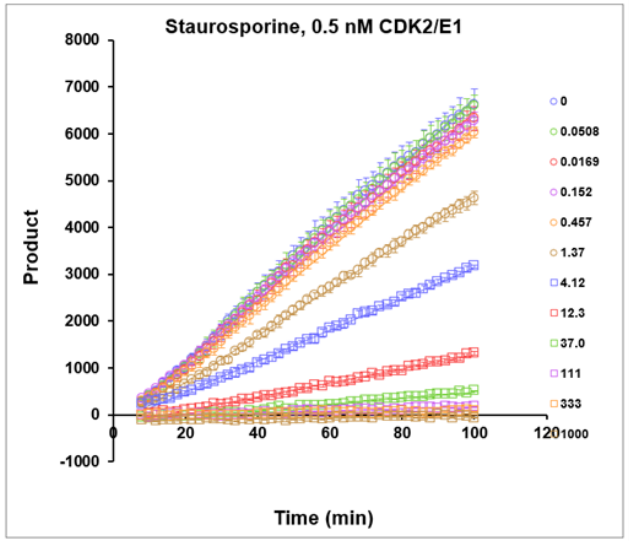

IC_{50} Curve

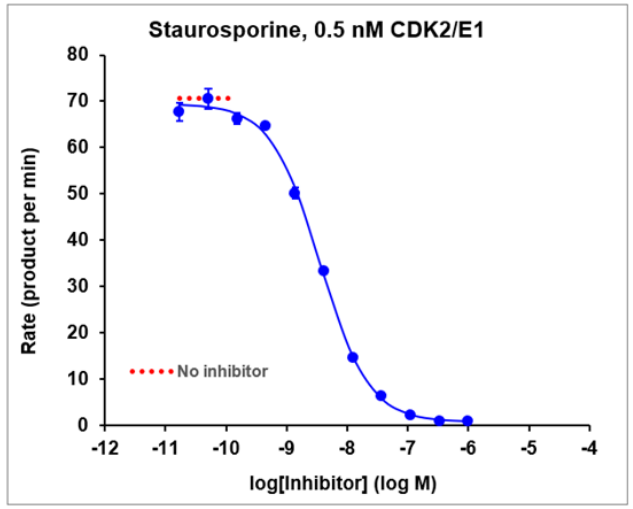

IC_{50} Table

Parameter	Value
Bottom	0.7
Top	69.5
log IC50	-8.44
IC50 (nM)	3.60
Ki (nM)	1.80
Slope	-1.081
R squared	0.999
IC50 approx SE (nM)	0.00
50% inhibition (nM)	3.67

The Y-axis label is RFU/min.


Staurosporine IC_{50} Determination at ATP K_m is 3.6 nM

Summary

Assay Validation Results and Progress Curve and Assay Strength at 1 mM ATP

Experiment	Result
Enzyme Titration Linear Range	0.04 - 0.31 nM
Sensor Peptide K_m Value	30 µM
ATP K_m Value	80 µM
DMSO Tolerance (highest % recommended)	2
Staurosporine IC50 Determination at ATP Km	3.6 nM

Progress Curve

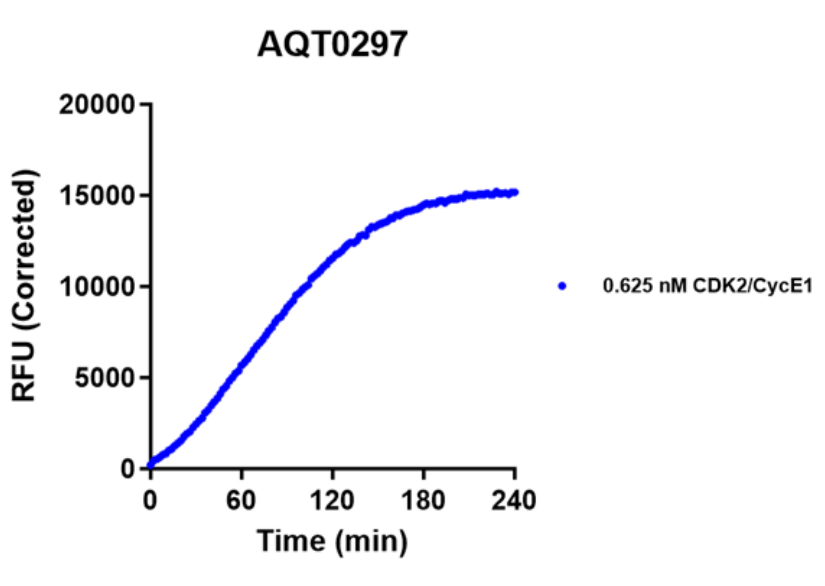

Kinase Name	Conc. (nM)	Sox-based Substrate Name	Normalized Reaction Rate (RFU/pmole/min)	Normalized Rate StndError (RFU/pmole/min)
CDK2/CycE1	0.625	AQT0297	16,928	56

Assay Strength Key	
Very Strong	>1,000 (RFU/pmole/min)
Strong	300 to 999 (RFU/pmole/min)
Moderate	100 to 299 (RFU/pmole/min)
Weak	30 to 99 (RFU/pmole/min)

Under the conditions utilized for this experiment, the assay is Very Strong